

# Metabolomics 101


UAB Metabolomics Training Course  
July 17-21, 2017

Wimal Pathmasiri and Delisha Stewart  
NIH Eastern Regional Comprehensive Metabolomics Resource Core  
(ERCMRC)  
Department of Nutrition – Nutrition Research Institute  
University of North Carolina at Chapel Hill

# Metabolomics

- The metabolome is the low molecular weight complement of cells, tissues, or biological fluids.
- Metabolomics investigations generally employ NMR or one of a number of types of chromatography coupled MS methods
- Metabolomics makes it feasible to uniquely profile the biochemistry of an individual, or model, apart from, or in addition to, the genome.
- Metabolomics is being used to reveal biomarkers for the early detection and diagnosis of disease, to predict outcomes, monitor therapeutic treatments and interventions, and to provide insights into biological mechanisms.


# The relation of proteins and metabolites to the genome



## DNA

DNA contains genetic instructions to


- make components of cells
- regulate the use of these components



## Proteins

Proteins are made of sequences of amino acids; the sequence defined by the gene.

Proteins are the enzymes that catalyze or accelerate chemical reactions in metabolism



## Metabolites

Metabolites are intermediates and products of metabolism.

**Catabolism:** the processes to breaks down large molecules.



**Anabolism:** the process to use catabolism energy to synthesize molecules

# Cells, Tissues, and Noninvasive Fluids



Cells / Organ

System

Released metabolites



Cytosolic metabolites




Serum  
Urine  
Saliva  
Breath  
Feces


*Signatures or Profiles*

*Discrete peaks* ⇒ *Diagnostics*


# NIH Eastern Regional Comprehensive Metabolomics Resource Core at NRI



## LC-MS, MS/MS and ION-MOBILITY





NMR




GC-MS


ICP-MS



## Multivariate and Statistical Analysis



## Predictive Modeling

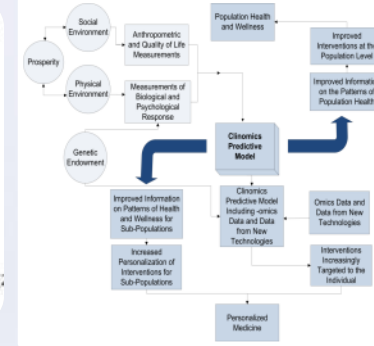


## Pathway Mapping Metabolites-Proteins-Genes




T  
A  
R  
G  
E  
T  
E  
D

B  
R  
O  
A  
D  
S  
P  
E  
C  
T  
R  
U  
M



# ERC/MRC Metabolomics Technologies

The analysis of the small molecule diversity present in a biological system and the pattern of changes arising from disease, dysfunction, disorder, or from the therapeutic or adverse effects of drugs.

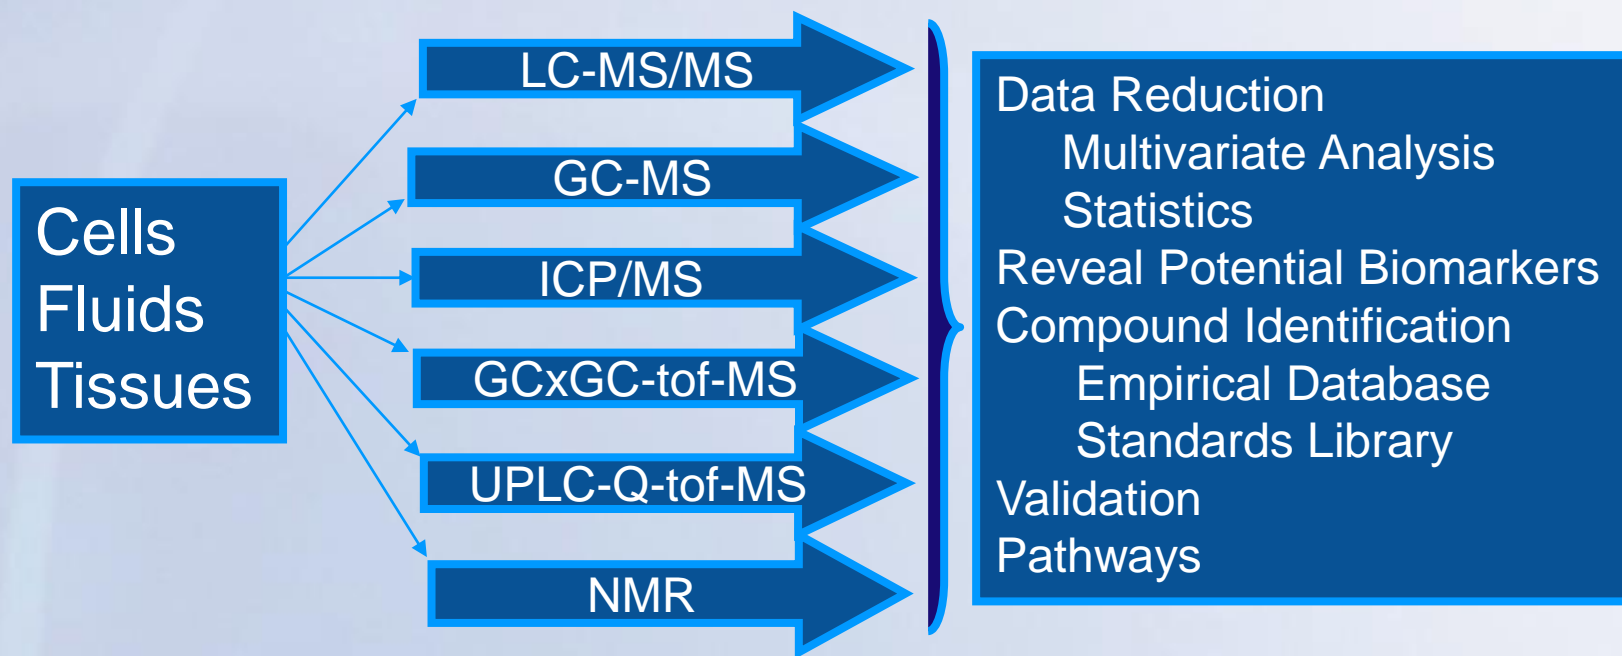

~6,500 discrete small molecule metabolites, ~ 25,000 genes, ~100,000 transcripts, and 1,000,000 proteins

# Optimal and Minimal Sample Volumes




	Minimum sample for MS Based Detection	Minimum Sample for NMR-Based Detection	Optimal Sample
Serum	50 ul	100 ul	1 ml
Urine	50 ul	200 ul	1 ml
Feces	20 mg	20 mg	500 mg
Tissue	50 mg	100 mg	500 mg
Cells	$1 \times 10^6$	$1 \times 10^7$	$1 \times 10^7$

# Cells, Tissues, and Noninvasive Fluids

Serum

Liver

Urine

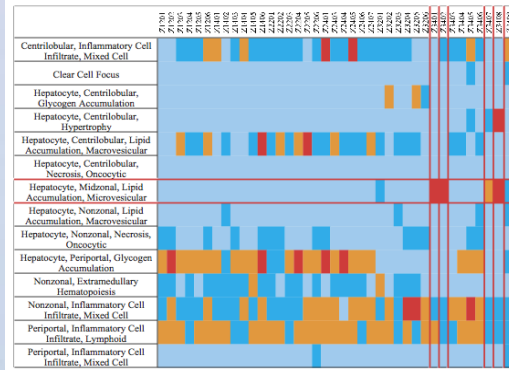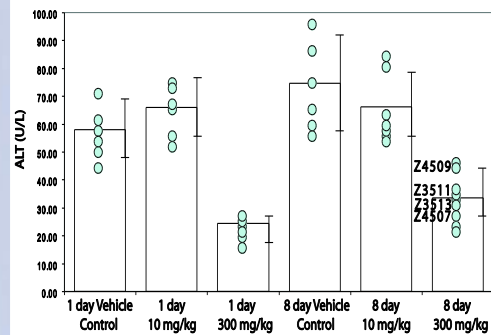




# Preclinical: Monitoring for Adverse Side Effects: DILI

- Drug-induced liver injury (DILI) accounts for 80% of the drug failure rate: pre-clinical through post market.
- Non-invasive markers are needed to determine the potential for DILI during treatment.
- Patients taking the anti-TB drug, isoniazid (INH), are at risk for developing liver injury. INH is one of the five top drugs with causal relation to liver injury and transplant in the US.
- Rats were dosed with INH for 1 or 8 days at low dose 'no affect' levels and at concentrations that resulted in microvesicular lipid accumulation (MVLA) of the liver- a reversible pathology currently diagnosed by biopsy and pathology.
- Metabolomics was used to determine urinary markers to correlate with MVLA diagnosis and its onset.


# Cells, Tissues, and Noninvasive Fluids

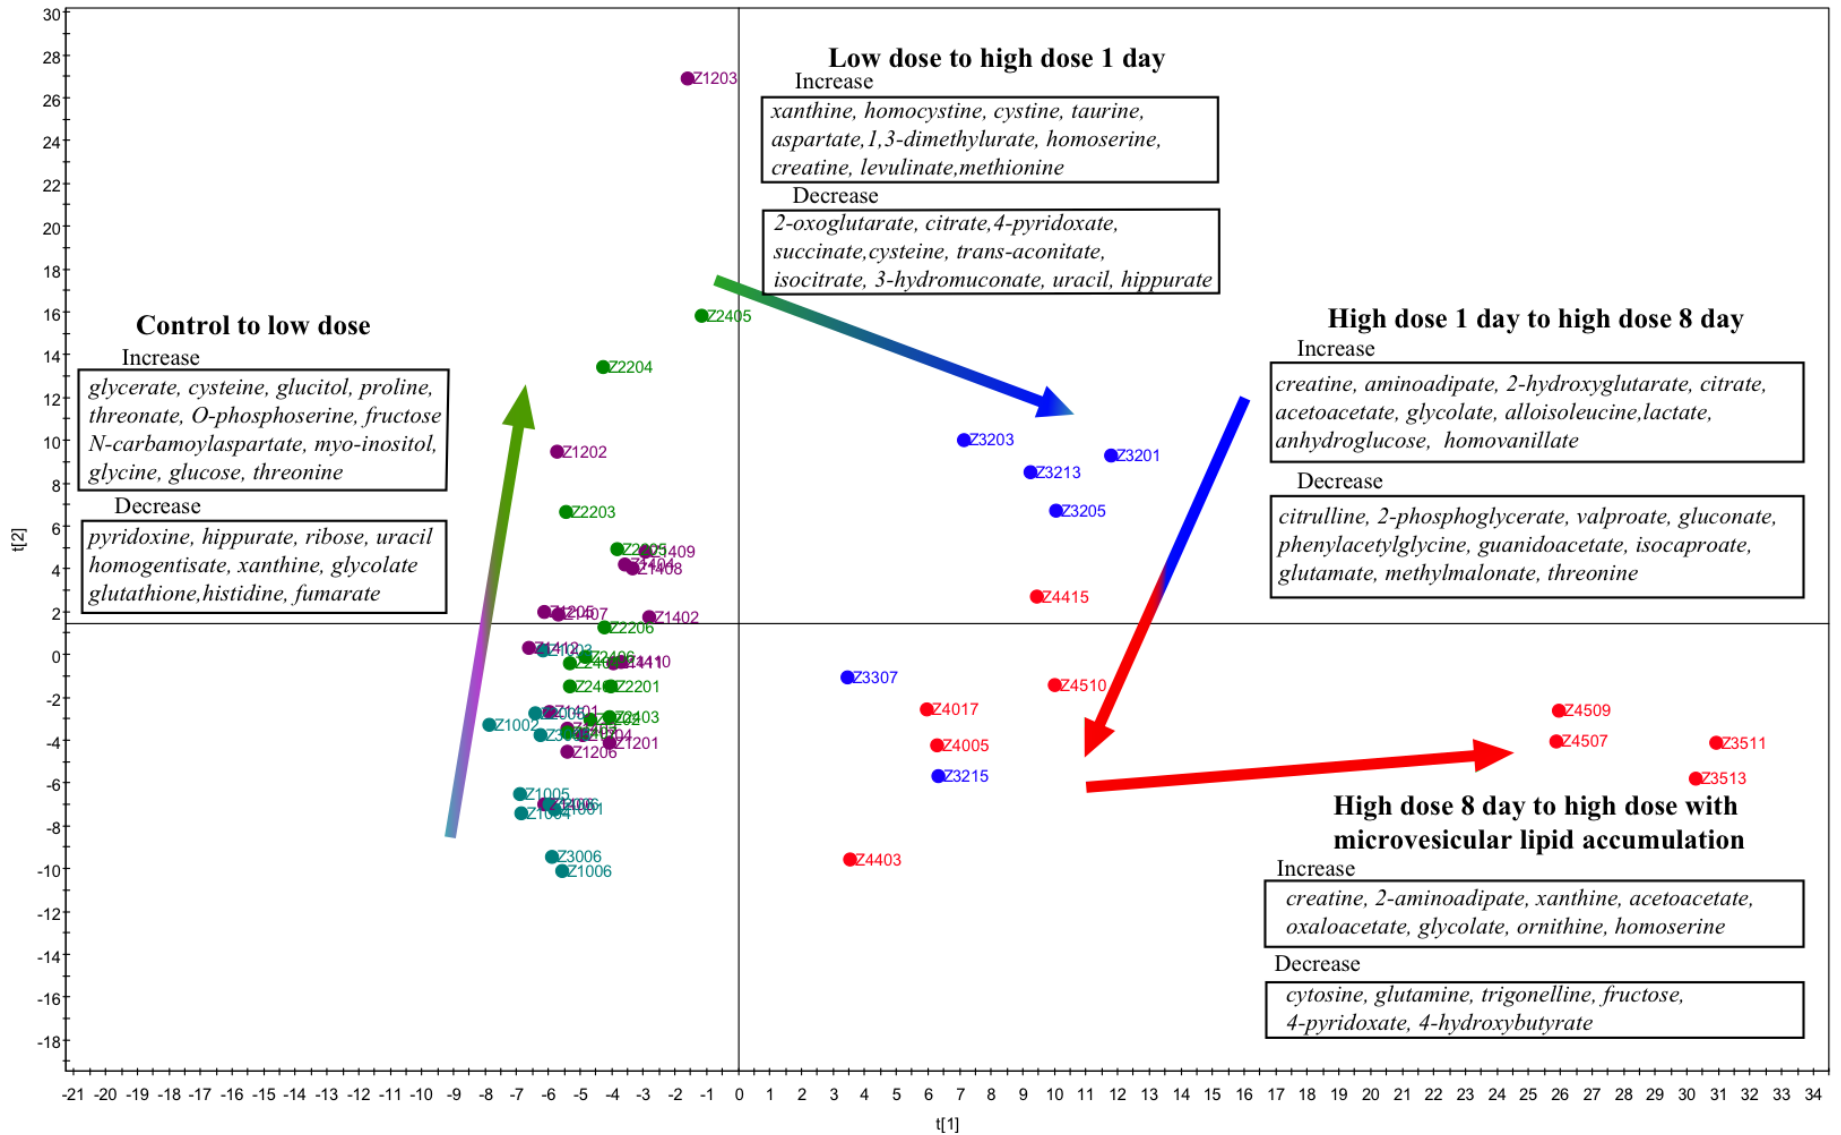





# NMR Based Metabolomics Analysis

- **NMR Spectroscopy**
  - A robust, reliable, and highly reproducible technique in metabolomics analysis
  - Quantitative and non-destructive method
  - Most labs use 600 – 950 MHz Spectrometers
  - The higher the field strength, the higher the sensitivity and resolution
- **Broad-spectrum metabolomics**
  - NMR binning (high throughput)
- **Targeted metabolomics**
  - Metabolite profiling and quantification of selected metabolites or a panel of metabolites

# NMR Metabolomics Workflow



Sample No.	Sample Name	Sample Type	Sample Volume (µL)	Sample Concentration (mg/mL)	Sample Weight (mg)	Sample Volume (µL)	Sample Concentration (mg/mL)	Sample Weight (mg)	Sample Volume (µL)	Sample Concentration (mg/mL)	Sample Weight (mg)	Sample Volume (µL)	Sample Concentration (mg/mL)	Sample Weight (mg)
1	Sample 1	Sample 1	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000
2	Sample 2	Sample 2	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000
3	Sample 3	Sample 3	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000
4	Sample 4	Sample 4	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000
5	Sample 5	Sample 5	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000
6	Sample 6	Sample 6	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000
7	Sample 7	Sample 7	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000
8	Sample 8	Sample 8	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000
9	Sample 9	Sample 9	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000
10	Sample 10	Sample 10	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000
11	Sample 11	Sample 11	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000
12	Sample 12	Sample 12	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000
13	Sample 13	Sample 13	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000
14	Sample 14	Sample 14	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000
15	Sample 15	Sample 15	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000
16	Sample 16	Sample 16	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000
17	Sample 17	Sample 17	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000
18	Sample 18	Sample 18	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000
19	Sample 19	Sample 19	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000
20	Sample 20	Sample 20	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000
21	Sample 21	Sample 21	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000
22	Sample 22	Sample 22	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000
23	Sample 23	Sample 23	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000
24	Sample 24	Sample 24	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000
25	Sample 25	Sample 25	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000
26	Sample 26	Sample 26	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000
27	Sample 27	Sample 27	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000
28	Sample 28	Sample 28	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000
29	Sample 29	Sample 29	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000
30	Sample 30	Sample 30	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000
31	Sample 31	Sample 31	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000
32	Sample 32	Sample 32	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000
33	Sample 33	Sample 33	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000
34	Sample 34	Sample 34	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000
35	Sample 35	Sample 35	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000
36	Sample 36	Sample 36	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000
37	Sample 37	Sample 37	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000
38	Sample 38	Sample 38	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000
39	Sample 39	Sample 39	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000
40	Sample 40	Sample 40	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000	100	1.0000	0.1000

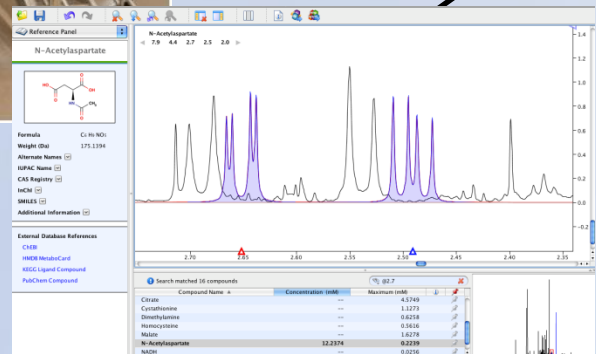

NMR data acquisition is performed by using methods cited in Beckonert et al. (2007), *Nature Protocols*, 2 (11), 2692-2703.

# Important Steps

- Study design
  - Match for factors such as gender, ethnicity, age, BMI (human studies)
  - Use of same strains in animal studies
- Sample collection
  - Collection vials, anticoagulant use (heparin, citrate, EDTA)
- Sample storage
  - -20 °C, -80 °C, minimize freeze-thaw cycles
- Sample preparation
  - Optimize the methods and use them consistently throughout study
  - Daily balance and pipette checks
- Use of Quality Check (QC) samples
  - Pooled QC samples (Phenotypic and combined pooled samples)
  - Use matching external pooled QC samples where pool samples cannot be prepared from study samples
- **Consistency and reproducibility are the keys for a successful metabolomics study**

# Sample Preparation for Metabolomics Analysis

Current sample preparation practices (in brief)

- **Biofluids**

- Dilute with D<sub>2</sub>O/ buffer/ 0.9% Saline
- Add internal standard (ISTD, eg. Chenomx) solution or formate (for serum).
- Centrifuge and transfer an aliquot into NMR tube

- **Tissue and Cells**

- Homogenization performed in ice cold 50/50 acetonitrile/water
- Supernatant dried down (lyophilized)
- Reconstituted in D<sub>2</sub>O and ISTD (eg. Chenomx) solution

- **Pooled QC Samples (Sample Unlimited)**

- Mix equal volume of study samples to get pooled QC samples
- 10% QC samples


- **Pooled QC Samples (Sample Limited)**

- Use independent pool of similar samples
- 10% QC samples


- **Daily balance and pipette check**

**Samples are randomized for preparation and data acquisition**

# Pooled QC Samples



- Aliquots from each sample in the study phenotype are pooled (phenotypic pool)
- Equal amount of each phenotypic pools are pooled (Combined phenotypic pool)
- Replicates of pools are prepared
- Pool samples are prepared along with the study samples




**Pooled samples  
should cluster tightly**

# NMR Data

- A typical  $^1\text{H}$  NMR Spectrum consists of thousands of sharp lines or signals.
- The intensity of the peak is directly related to the number of protons underlying the peak.
- The position of a particular peak in the X-axis of the NMR spectrum is called the “Chemical Shift” and it is measured in ppm scale
- The NMR spectrum obtained for the biological sample is referenced using a reference compound such as DSS, TSP, or Formate added to the sample in sample preparation step.
- pH indicator may also be used (for example, Imidazole)



# $^1\text{H}$ NMR Spectrum for alanine

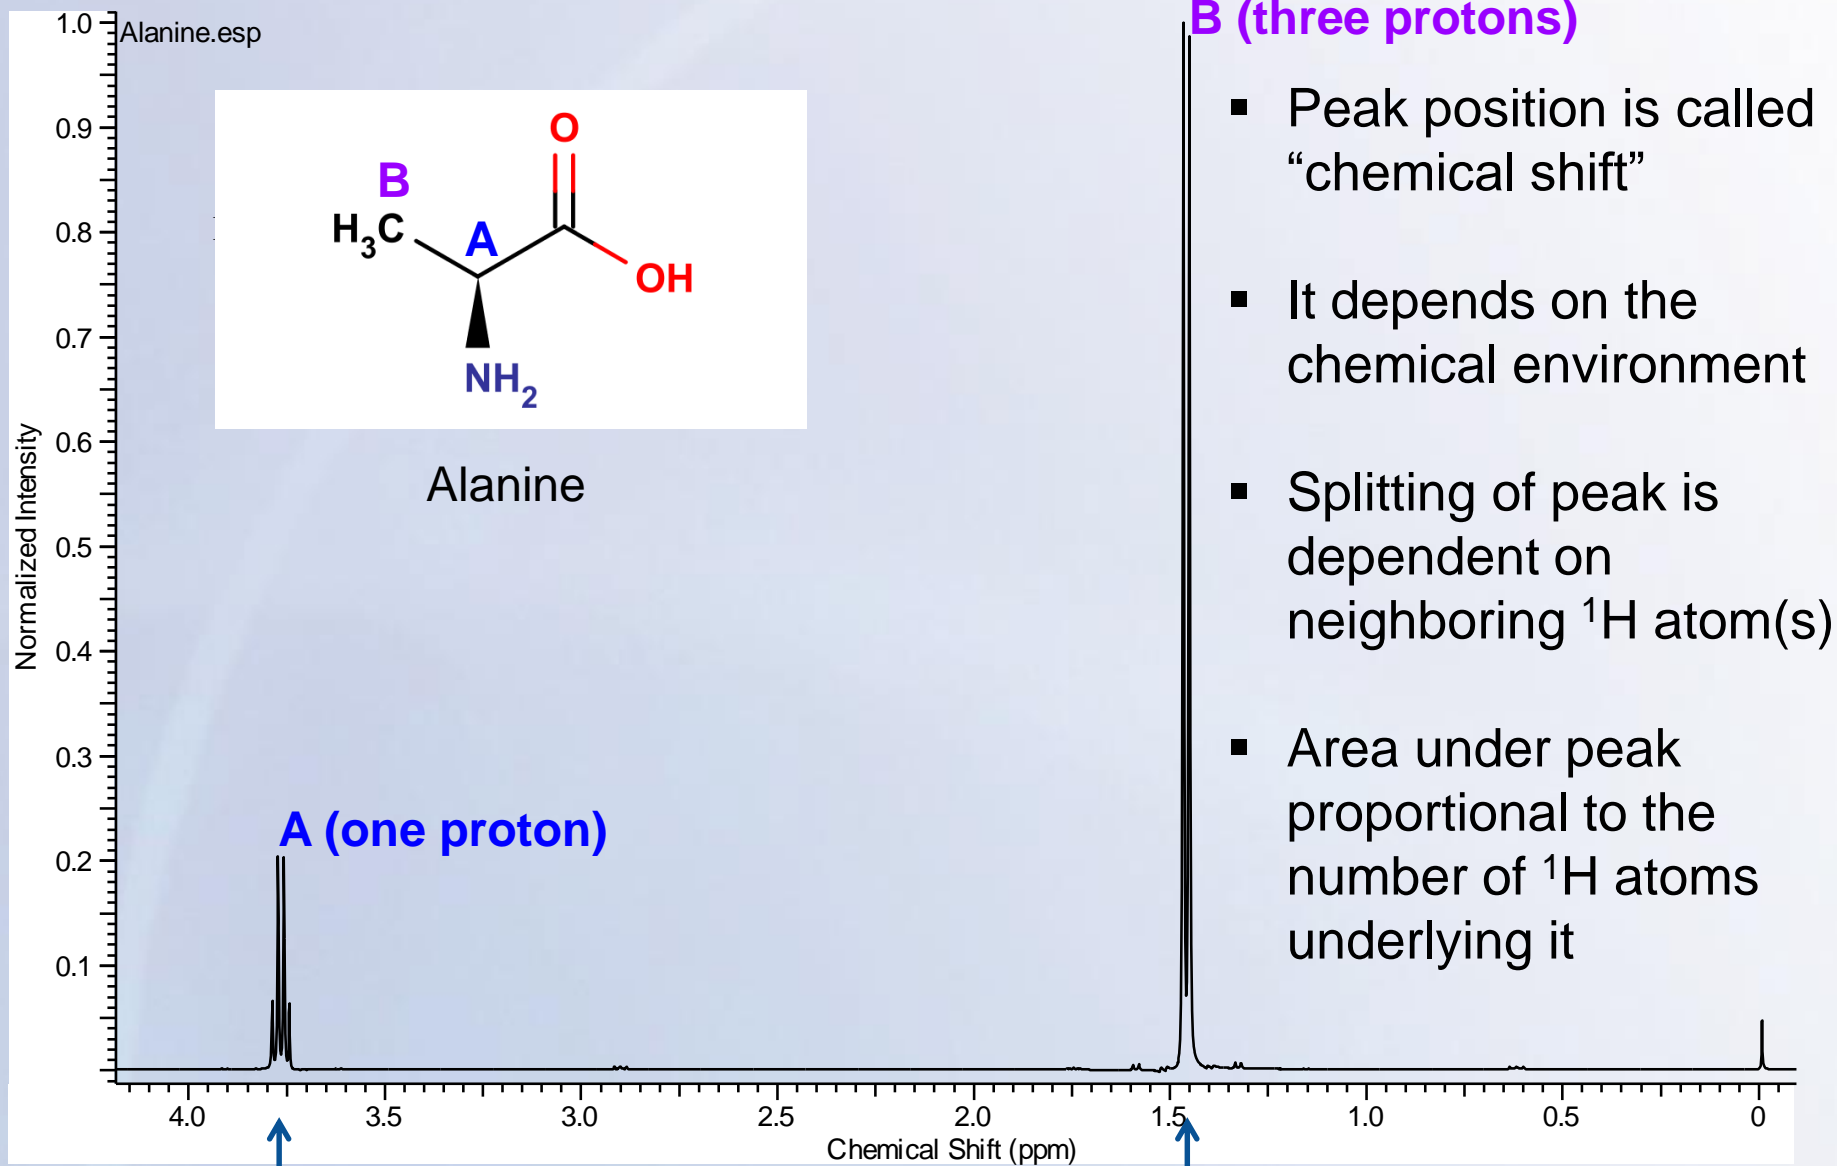


Chemical shift of  $\text{CH}$   
4 lines (quadrant)


Chemical shift of  $\text{CH}_3$   
2 lines (doublet)

- Peak position is called “chemical shift”
- It depends on the chemical environment
- Splitting of peak is dependent on neighboring  $^1\text{H}$  atom(s)
- Area under peak proportional to the number of  $^1\text{H}$  atoms underlying it

# Typical $^1\text{H}$ NMR Spectrum of urine





# Typical $^1\text{H}$ NMR Spectrum of Urine (annotated)



# Broad Spectrum Metabolomics NMR Binning

# Binning



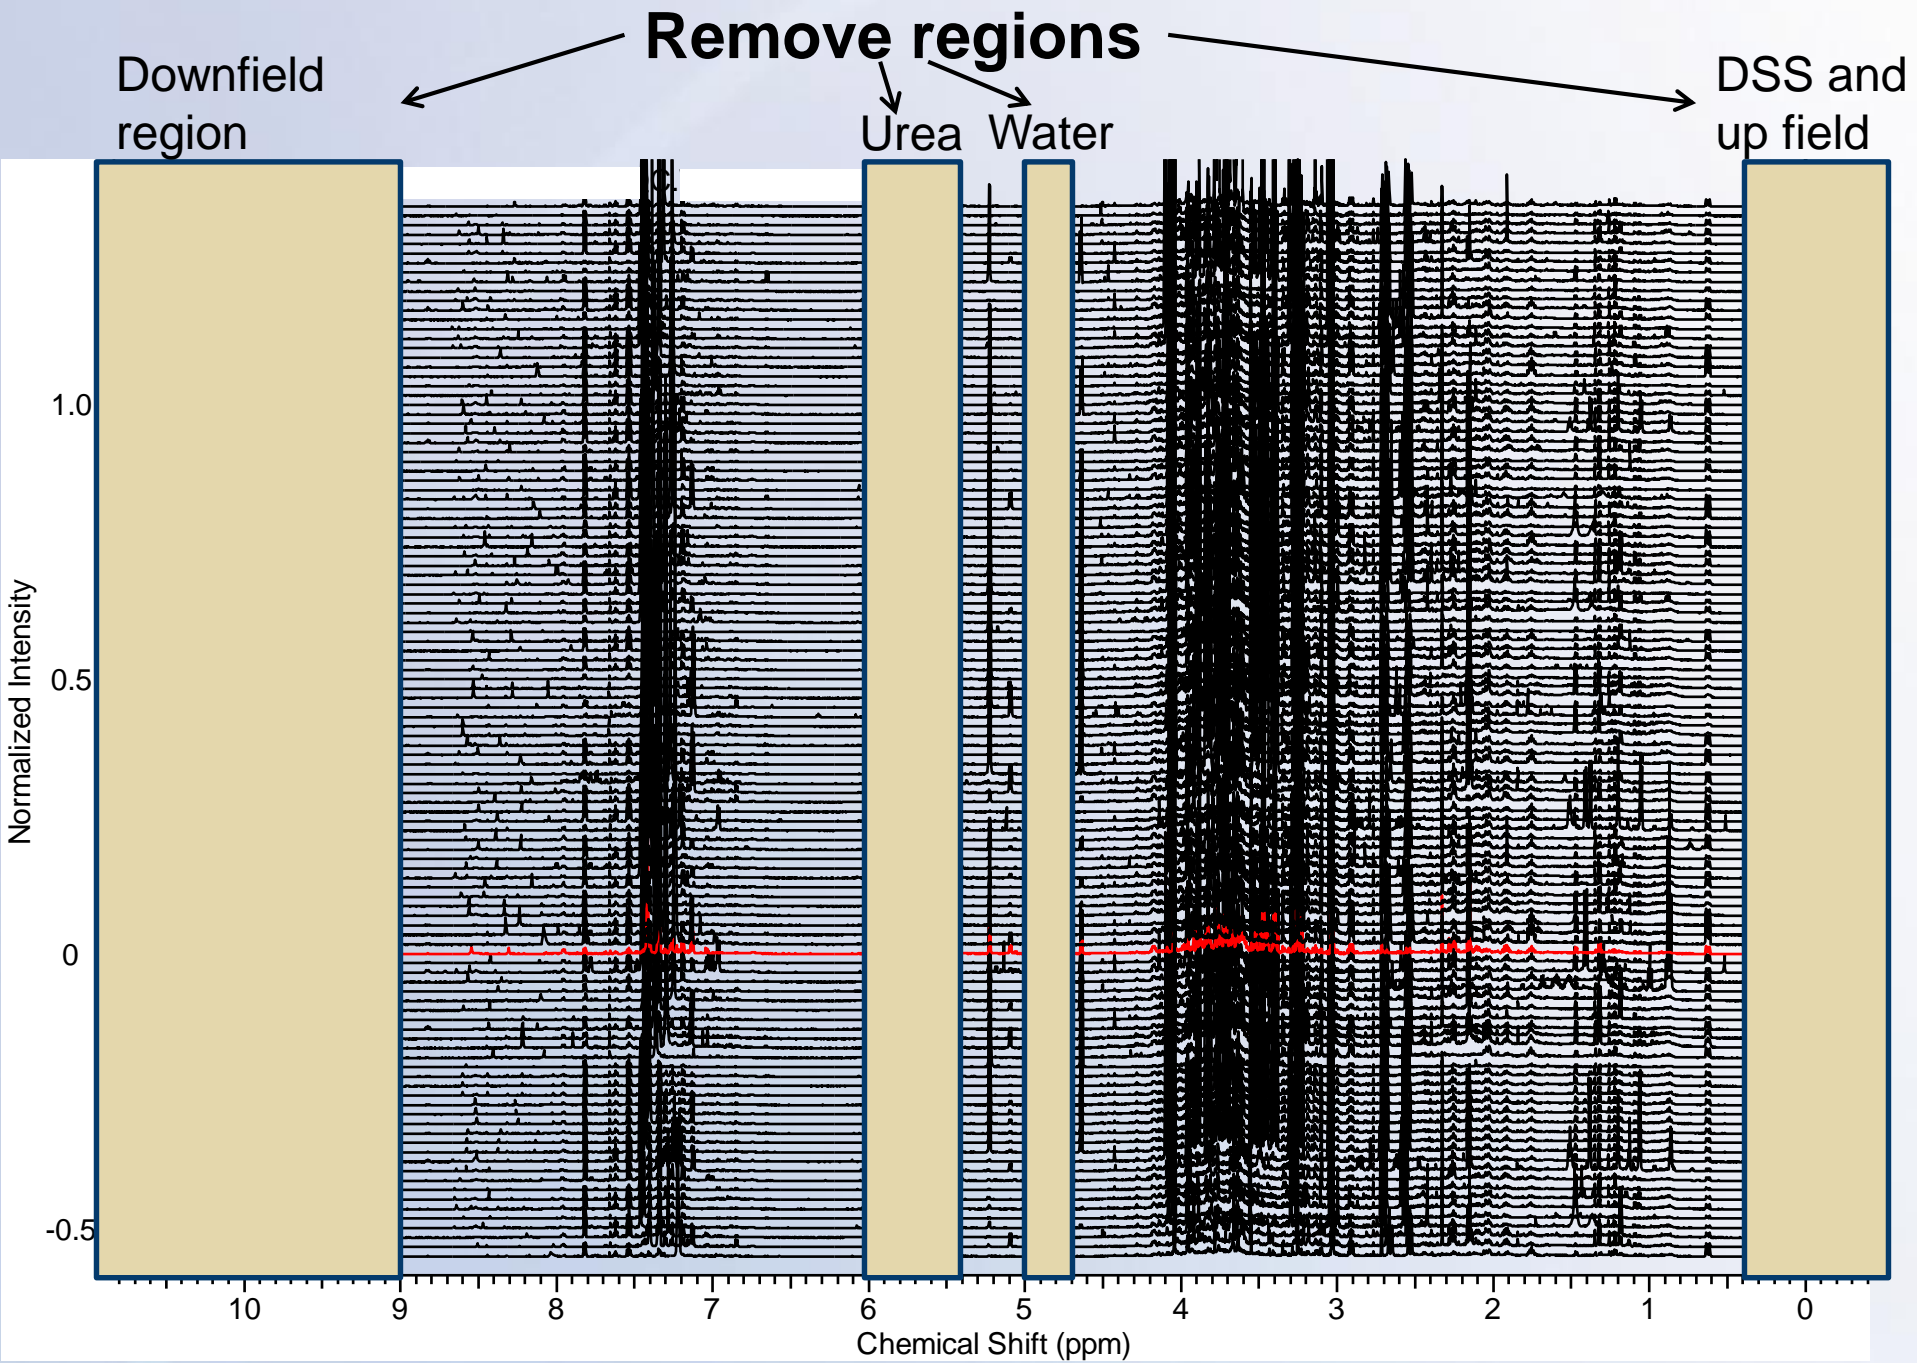

# Binning

- Integrate bins (0.04 ppm bin size)
- Normalize bins to the total integral of each spectrum
- Merge metadata
- Result is a spreadsheet ready for further multivariate data analysis and other statistical analysis




Sample ID	Disease Group	[0.40 .. 0.46]	[0.46 .. 0.52]	[0.52 .. 0.54]	[0.54 .. 0.57]	[0.57 .. 0.60]	[0.60 .. 0.66]	[0.66 .. 0.68]	[0.68 .. 0.71]	[0.71 .. 0.75]
C0559	Cases	7.60E-05	0.00E+00	7.32E-02	8.48E-02	3.20E-02	1.84E+00	1.31E-01	3.60E-01	3.67E-01
C0629	Cases	0.00E+00	1.78E-02	0.00E+00	2.18E-02	0.00E+00	1.08E+01	0.00E+00	0.00E+00	3.02E-02
C0640	Cases	3.44E-04	0.00E+00	1.83E-03	1.86E-04	0.00E+00	4.51E+00	0.00E+00	0.00E+00	0.00E+00
C0835	Cases	6.41E-04	0.00E+00	6.44E-03	0.00E+00	3.96E-03	3.28E+00	0.00E+00	5.12E-03	1.75E-02
D0613	Cases	6.63E-03	0.00E+00	0.00E+00	1.06E-02	0.00E+00	5.79E+00	0.00E+00	6.36E-02	3.02E-01
D0762	Cases	0.00E+00	0.00E+00	1.79E-02	1.98E-02	0.00E+00	9.37E+00	0.00E+00	0.00E+00	1.74E-02
D1113	Cases	3.14E-03	2.42E-03	8.02E-02	1.04E-01	5.32E-03	3.74E+00	0.00E+00	2.02E-02	1.84E-01
D1158	Cases	0.00E+00	3.71E-03	2.35E-02	4.83E-02	0.00E+00	5.02E+00	0.00E+00	1.91E-02	0.00E+00
D2090	Cases	0.00E+00	0.00E+00	2.45E-03	9.98E-04	0.00E+00	5.76E+00	0.00E+00	1.24E-02	1.04E-02
E0004	Cases	1.72E-03	0.00E+00	6.85E-02	3.05E-02	0.00E+00	1.47E+00	6.90E-02	3.61E-01	4.08E-01
E0195	Cases	0.00E+00	1.69E-03	5.57E-02	6.29E-02	0.00E+00	2.77E+00	1.34E-01	2.04E-01	4.56E-01
E0225	Cases	1.25E-03	0.00E+00	4.40E-03	1.69E-02	0.00E+00	9.17E+00	0.00E+00	1.08E-02	2.30E-02
E0309	Cases	4.11E-03	0.00E+00	2.23E-02	7.54E-03	3.08E-03	3.54E+00	0.00E+00	3.28E-02	9.09E-01
E0487	Cases	1.72E-03	0.00E+00	0.00E+00	1.00E-02	0.00E+00	4.00E+00	0.00E+00	1.36E-02	0.00E+00
F0036	Cases	1.66E-02	0.00E+00	0.00E+00	2.06E-02	0.00E+00	1.22E+01	1.04E-02	0.00E+00	5.97E-01
F0108	Cases	0.00E+00	2.31E-03	6.30E-03	1.11E-02	0.00E+00	7.17E+00	0.00E+00	1.65E-02	2.21E-01
A0233	Control	0.00E+00	1.86E-02	0.00E+00	1.82E-02	0.00E+00	1.61E+01	0.00E+00	2.91E-03	0.00E+00
A0490	Control	0.00E+00	0.00E+00	2.99E-03	3.60E-02	0.00E+00	2.97E+00	0.00E+00	4.00E-02	5.46E-01
A2003	Control	0.00E+00	0.00E+00	3.45E-02	2.20E-02	0.00E+00	1.80E+00	0.00E+00	0.00E+00	0.00E+00
C0586	Control	0.00E+00	1.69E-02	0.00E+00	6.64E-03	0.00E+00	1.92E+01	0.00E+00	6.51E-02	0.00E+00
C2177	Control	0.00E+00	0.00E+00	3.02E-02	3.59E-02	0.00E+00	2.35E+00	0.00E+00	3.19E-02	1.49E-01
D0177	Control	9.21E-03	0.00E+00	1.69E-02	1.47E-02	0.00E+00	2.43E+00	0.00E+00	4.46E-02	0.00E+00
D0729	Control	0.00E+00	1.88E-03	5.58E-02	7.87E-02	2.92E-02	3.16E+00	6.59E-02	2.80E-01	4.30E-01
D0909	Control	0.00E+00	1.08E-03	0.00E+00	5.69E-03	0.00E+00	2.49E+00	0.00E+00	1.01E-02	1.87E-01
D0945	Control	0.00E+00	4.79E-04	7.00E-03	0.00E+00	4.19E-03	3.99E+00	0.00E+00	1.11E-03	3.96E-02
D1174	Control	0.00E+00	9.33E-04	0.00E+00	3.43E-03	1.30E-02	7.21E+00	6.53E-03	0.00E+00	1.66E-02
D2054	Control	1.55E-03	0.00E+00	0.00E+00	1.22E-02	0.00E+00	2.07E+00	0.00E+00	1.28E-02	3.90E-01
D2062	Control	2.39E-05	0.00E+00	6.04E-02	2.99E-02	0.00E+00	4.94E+00	0.00E+00	9.95E-03	0.00E+00
D2079	Control	2.73E-02	0.00E+00	1.81E-03	1.17E-02	0.00E+00	3.38E+01	7.87E-02	0.00E+00	5.91E+00

# Multivariate Data Analysis & Other Statistical Analysis



# Multivariate data analysis and other statistical analyses


- Mean centered and scaled data
- Non-supervised analysis
  - Principal component analysis (PCA)
- Supervised analysis
  - PLS-DA and OPLS-DA
- Loadings plots and VIP Plots to identify discriminatory bins
- p-Value, fold change




# Library Matching (and quantifying) Using Chenomx




# chemical shift and pH dependence




# NMR Spectrum of Urine with Chenomx Library Fit of Metabolites




# Fitting of metabolites




# Fitting taurine



**Taurine**  
1.03 mM




# Fitting fucose







# Additive Fit

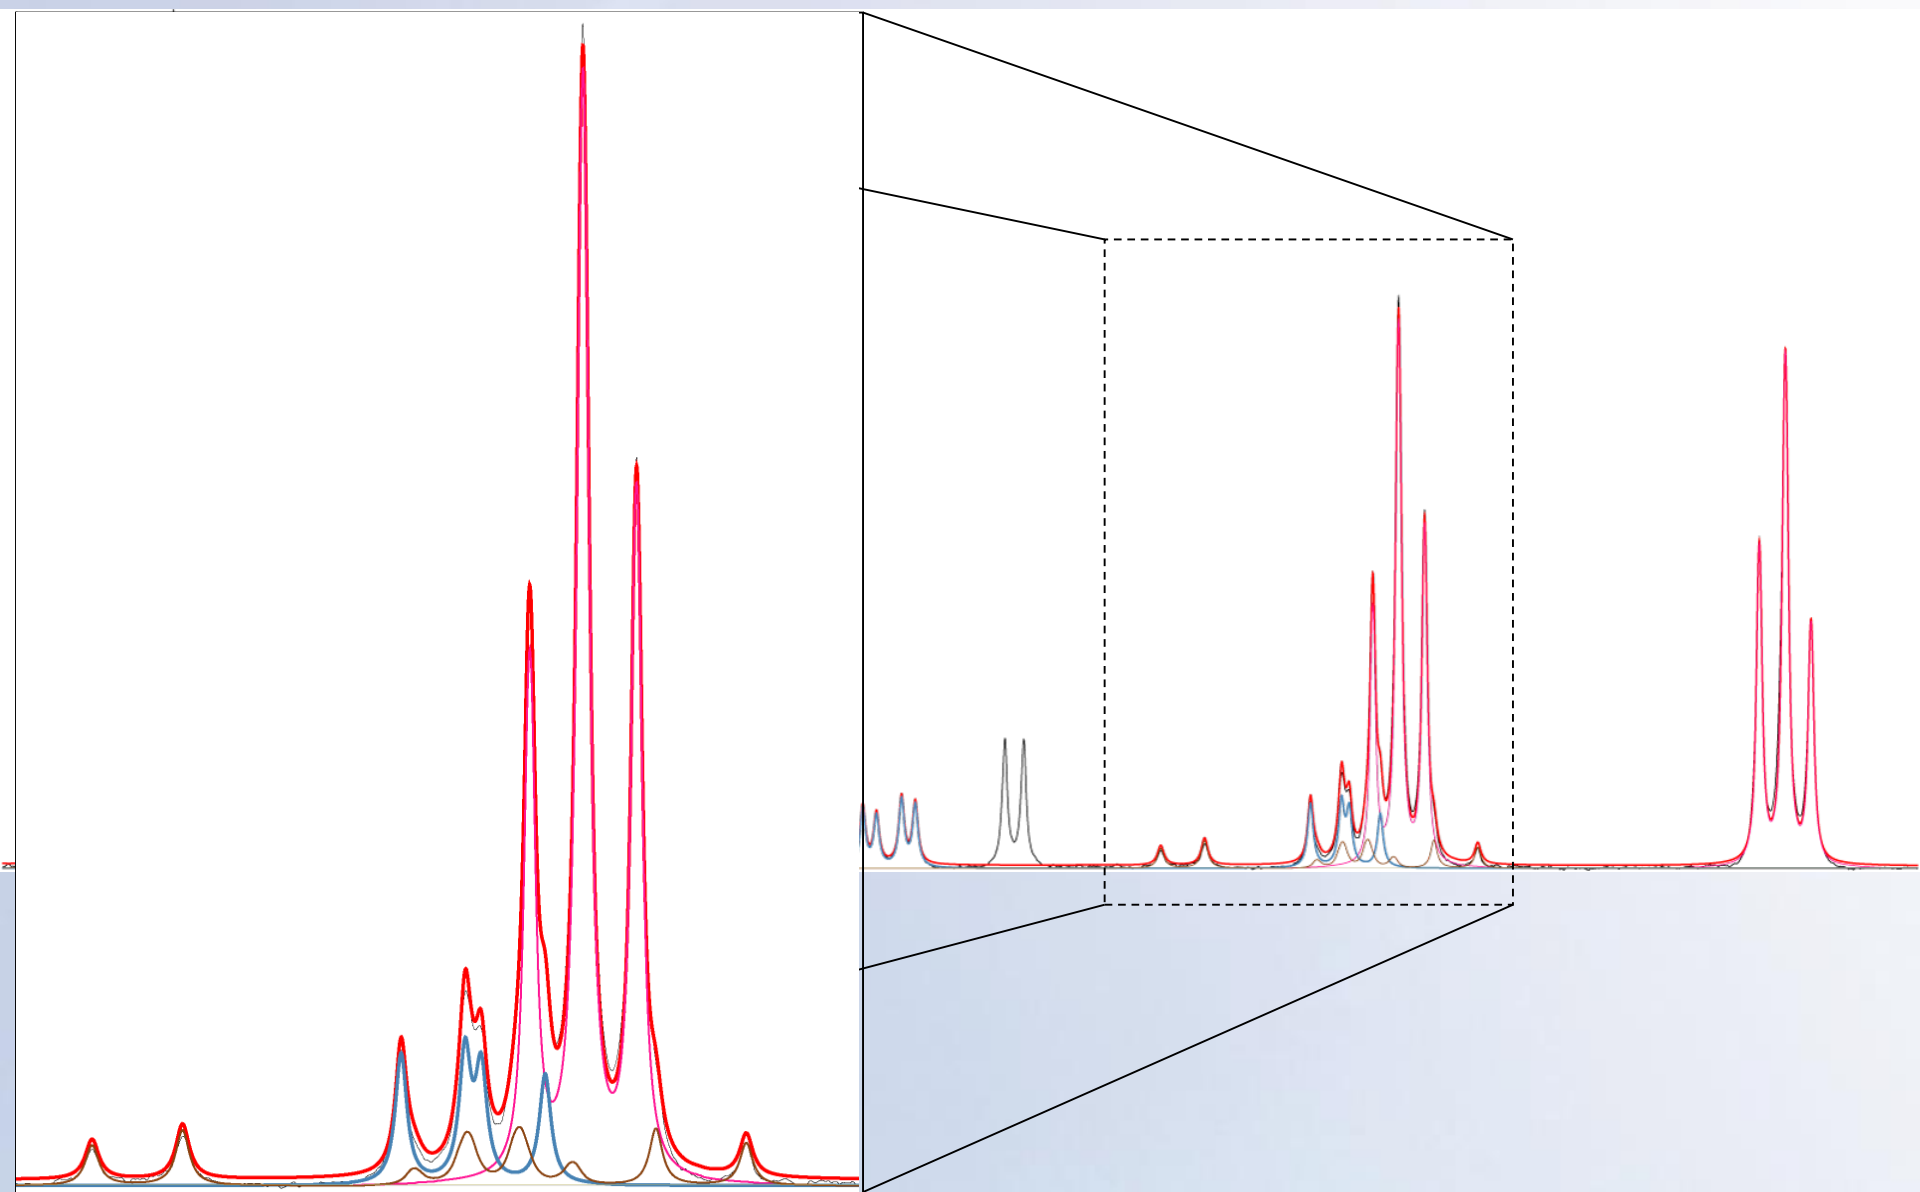

# Chenomx Helps Resolving Ambiguity in Highly Overlapped Regions



# Additive fit

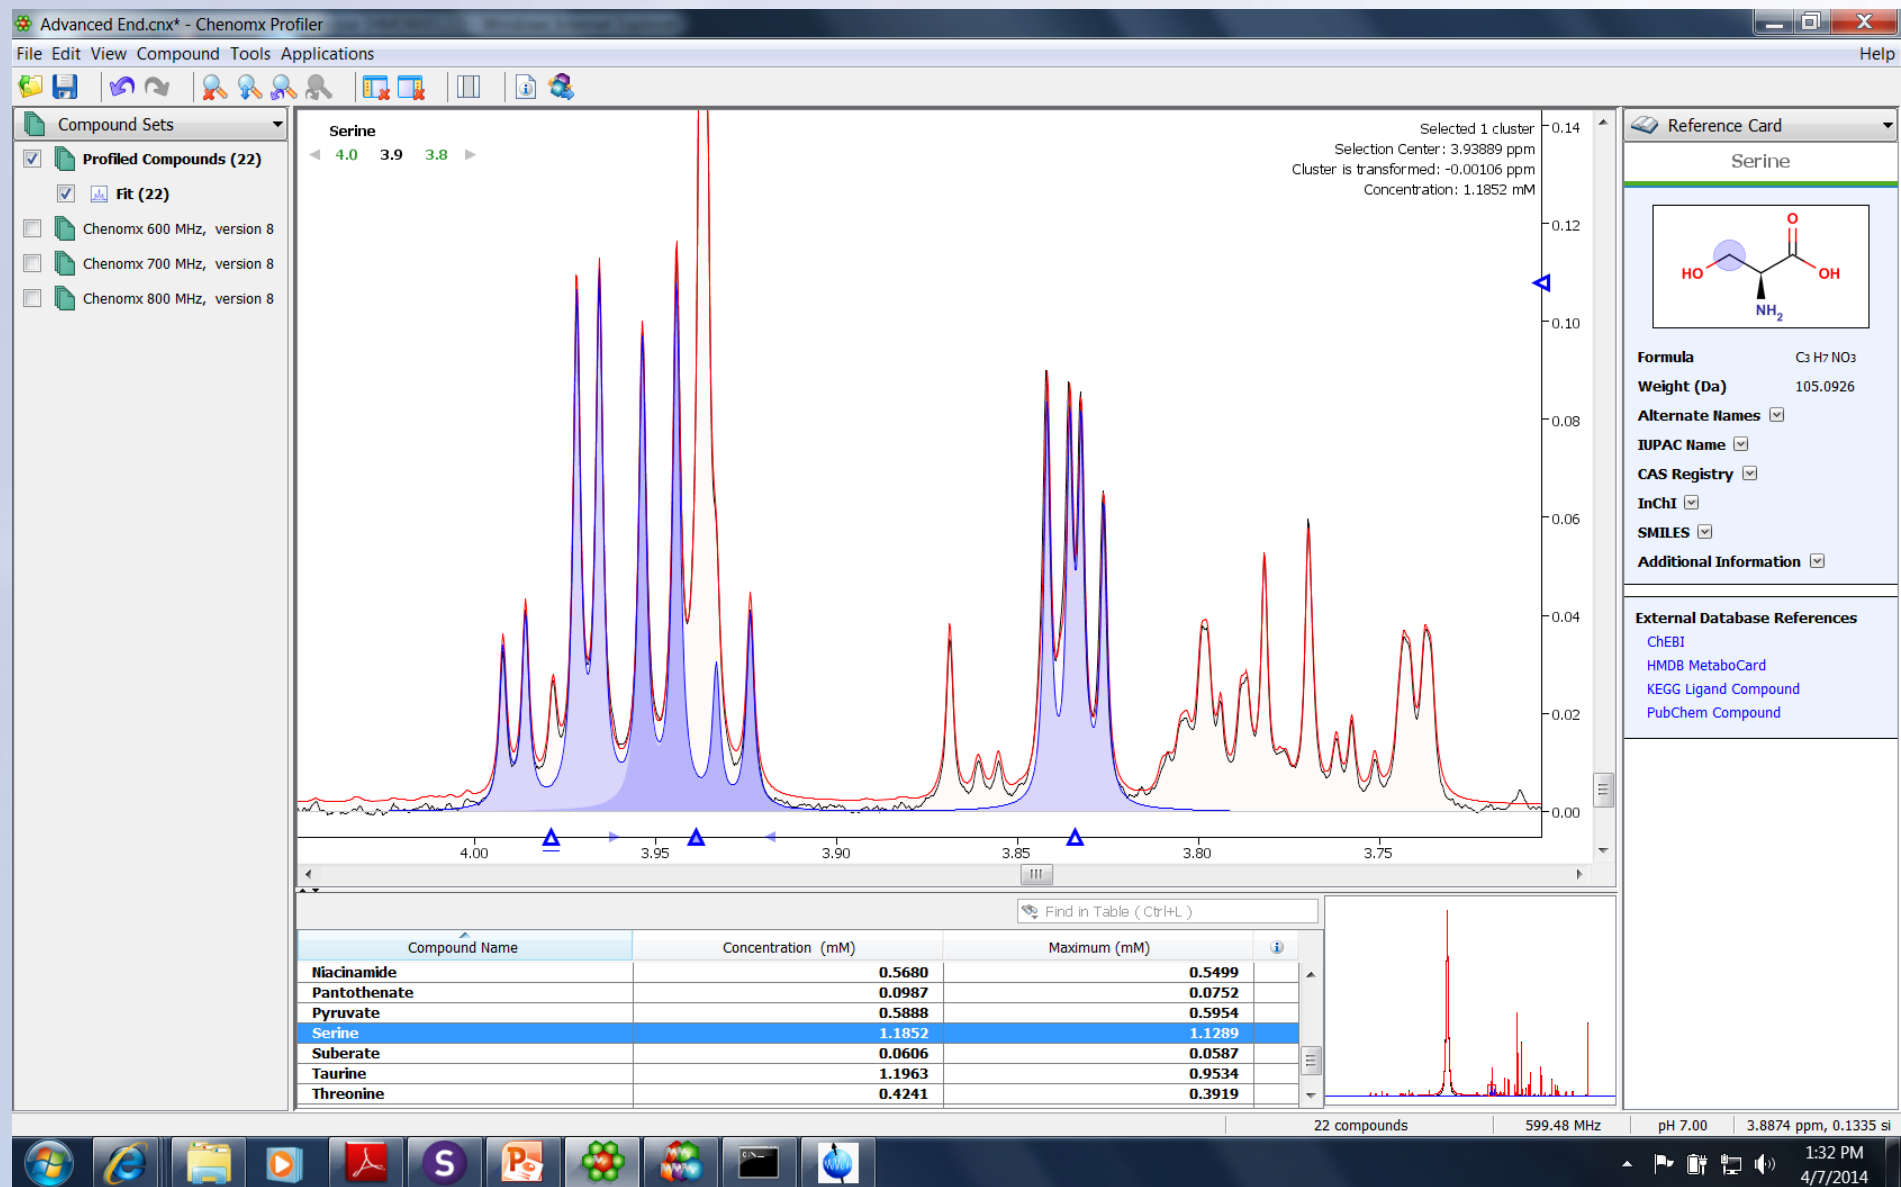

# Interpretation & Metabolic Pathway Analysis

# Interpreting results and Pathway Analysis

Once we have performed a metabolomics analysis,

- We find some important metabolites that are responsible for the separation of study groups.
- The next question is “What it means?”
- How do you correlate these finding to your study questions?
- Does it explain any findings that are meaningful for your study hypotheses?
- Does it generate a new hypothesis?
- How do you answer these questions?

Next step is to interpret results and  
metabolic pathway analysis


# Interpreting results and Pathway Analysis

- There is a number of freely available software
  - Metaboanalyst, MetScape 3 for Cytoscape, metaP-Server, web based KEGG Pathways.
- Another way of interpreting metabolomics results is to use traditional biochemistry text books.
- The input for pathway analysis is typically a list of metabolites (with any fold change or p-value information)
- Genomics, transcriptomics, and/or proteomics data can be integrated
- Once these pathways are identified, you may perform a targeted metabolomics analysis to validate the findings from global analysis.

# Day 0 serum- Predicting Day 28 Response to Vaccine

## PLS-DA

Day 0 – High Responders (Black) vs Low Responders (Red)



## Subset of Metabolites that Influence the Separation of Subjects at Day 0 (VIP ≥ 1 or p-value ≤ 0.1)

Isoleucine**	Creatinine**
Leucine**	Cysteine**
Valine	Histidine
3-Methyl-2-oxo-isovalerate	Choline
3-Hydroxybutyrate	Glucose
Lactate	Betaine
Alanine	TMAO
Acetate**	Glycine
Proline*	Glycerol
Glutamate**	Serine
Glutamine**	Creatine
Pyruvate	Tyrosine*
2-Oxoisocaproate	Histidine
Methylguanidine**	Tryptophan
Formate	Phenylalanine

\*p-value < 0.05, \*\*p-value ≤ 0.1

Preliminary results





# Some Software available for NMR Based Metabolomics

## FREE

- NMR Data Processing
  - ACD Software for Academics (ACD Labs, Toronto, Canada)
- Multivariate data analysis
  - MetaboAnalyst 3.0 (<http://www.metaboanalyst.ca>)
  - MetATT (<http://metatt.metabolomics.ca/MetATT/>)
  - MUMA (<http://www.biomolnmr.org/software.html>)
  - Other R-packages
- Library matching and Identification
  - Bayesil (<http://bayesil.ca/>, includes quantification)
  - BATMAN
  - Use of databases
    - Birmingham Metabolite library, HMDB, BMRB
- Pathway analysis
  - Metaboanalyst, MetScape 3 for Cytoscape, metaP-Server, KEGG

Also available through [www.metabolomicsworkbench.org](http://www.metabolomicsworkbench.org)

# Some Software available for NMR Based Metabolomics

## COMMERCIAL

- NMR Data-preprocessing
  - ACD Software (ACD Labs, Toronto, Canada)
  - Chenomx
- Multivariate data analysis
  - SIMCA 13
- Other statistical analysis
  - SAS, SPSS
- Library matching and quantification
  - Chenomx
- Pathway analysis
  - GeneGo (MetaCore Module)
  - Ingenuity Pathway Analysis (IPA)

# ERCMRC at UNC Chapel Hill



Yuanyuan Li  
LC-MS/MS  
LC-TOF-MS




Wimal Pathmasiri  
NMR & GC-TOF-MS




Delisha Stewart  
NMR and LC-TOF-MS



Maria Moreno  
NMR and LC-MS/MS



Reza Ghanbari  
Postdoctoral Fellow



Rose Ewald  
Graduate Studies



Susan Sumner  
PI, ERCMRC



Susan McRitchie  
Program Coordinator  
Data Analysis

## NCRC



Nick Gillitt  
Dole  
700 MHz NMR  
6500 Sciex LC-MS



Colin Kaye  
NCSU  
6500 Sciex  
Triple Quad



UNC-G  
Q-Exactive



Debby Reed  
GC-MS  
GC-TOF-MS



Stephen Orena  
LC-MS/MS



Martin Kohlmeier  
Training



Tim Fennell  
Director,  
Analytical Chemistry &  
Pharmaceutics



Yan Lan Yueh  
LC-MS

## RTI



Jessica Gooding  
LC-MS



Rod Snyder  
NMR and LC-MS



Courtney Whitaker  
LC-MS

Scott Watson  
Neurotransmitter  
LC/MS

## DHMRI



Kevin Knagge  
700 and 950 MHz NMR

Jason Winnike  
NMR  
2D-GC-TOF-MS




David Kirchner  
LC-MS/MS




Huadong Chen  
LC-MS  
LC-TOF-MS

Huiyuan Chen  
GC-MS  
GC-TOF-MS



## UNC Charlotte Bioinformatics



Owen Myers



XiuXia Du

Aleksandr  
Smirnov

