


UAB
THE UNIVERSITY OF
ALABAMA AT BIRMINGHAM
Knowledge that will change your world

GBS 724
March 24, 2017

Real-time connection of Mass Spectrometry with Medicine and Surgery

Stephen Barnes, PhD
Professor of Pharmacology & Toxicology
Director, Targeted Metabolomics and
Proteomics Laboratory

T Targeted
M Metabolomics &
P Proteomics
L Laboratory

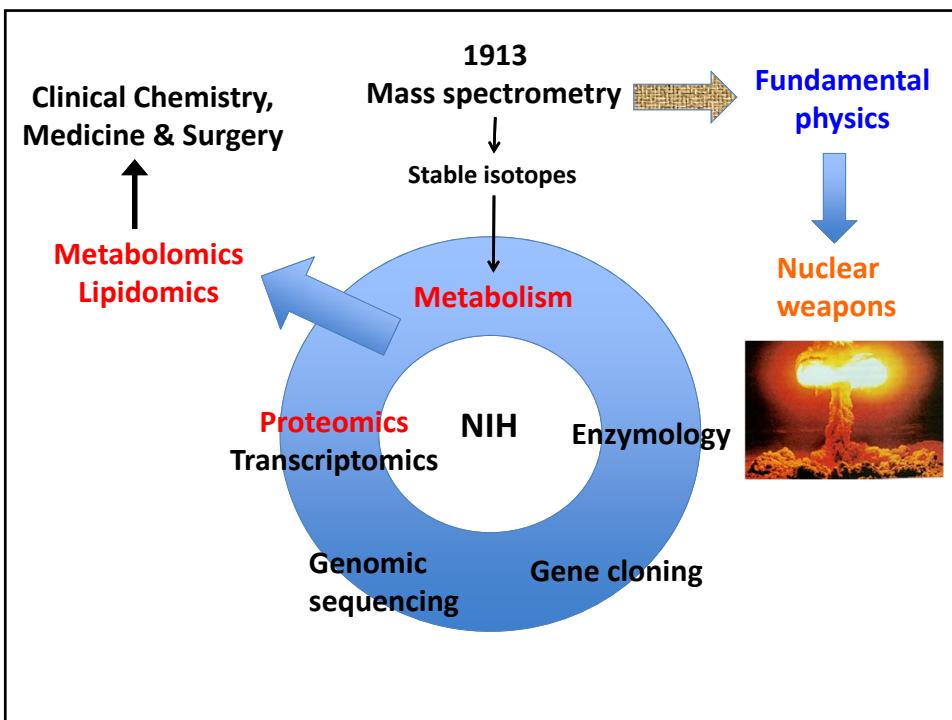

Dissociative research

- Samples are collected and stored for analysis at a “later” time
- “Later” can be months or years after sample collection
 - Of little direct benefit to the patient
 - Although may influence the community of patients
 - True of many analyses

Real time analysis

- Existing, familiar applications
- Gases!
- The iKnife
 - GI surgery
 - Cancer margins
 - Pathology
- DESI
- CARS

Real-time analysis


- We see the real-time use of MS when we go through security checks at the airport
 - Checks for ion signatures of explosives



- Other devices are used to check for specific volatiles in the breath



Noses and smell – real time analysis

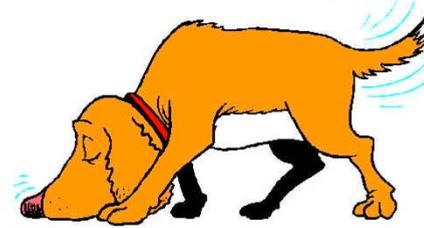

The superior volatile metabolite detector

Gases produced in the GI tract

- H₂, CO₂ and CH₄ from carbohydrates
 - Firmicutes
 - From pyruvate and NAD(P)H/FADH₂
 - H₂ used by sulfate-reducing bacteria (SRBs), methanogenic Archaea, and acetogens
- SRBs produce H₂S
- NO from nitrates

Methods for measuring gases

Technology	Operation mode	Target intestinal gas	Detection limit	Cross-sensitivity	Response time	Life time	Estimated cost
<i>Spectrometry based^a</i>							
GC-MS	Off line	All gases	ppt to ppb	Low	~Several minutes	Long	>US\$300k
IMS	Real time	All gases	ppb	Low	<1 min	Long	>US\$100k
PTR-MS	Real time	All gases	ppt	Low	<1 min	Long	>US\$400k
SIFT-MS	Real time	All gases	ppb	Low	<1 min	Long	>US\$400k
LS	Real time	Most gases except H ₂	ppt to ppb	Low	<1 min	Long	<US\$50k
<i>Sensor based^b</i>							
Electrochemical	Real time	H ₂ , H ₂ S, NO, and CO ₂	ppm	Medium	<30 s	Short	<US\$100
Calorimetric	Real time	H ₂ , CH ₄ , and CO ₂	ppt	High	<10 s	Medium	<US\$100
NDIR	Real time	CO ₂ , CH ₄ , and VOCs	ppm to ppt	Low	<20 s	Long	<US\$300

GC-MS gas chromatography-mass spectrometry

IMS ion mobility mass spectrometry


PTR-MS proton transfer reaction mass spectrometry

SIFT-MS selection ion flow tube-mass spectrometry

LS laser spectrometry


Jian Zhen Ou et al., Trends Biotech, 2015



Device for measuring fecal gas production

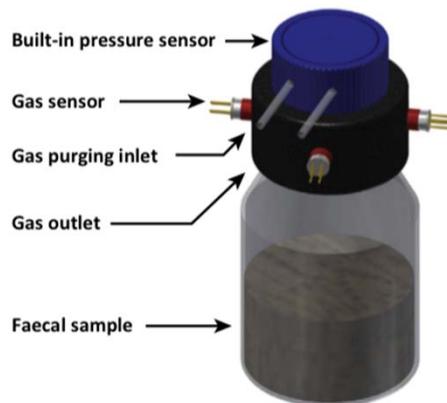

Jian Zhen Ou et al., Trends Biotech, 2015

Fecal gas production (ex vivo)

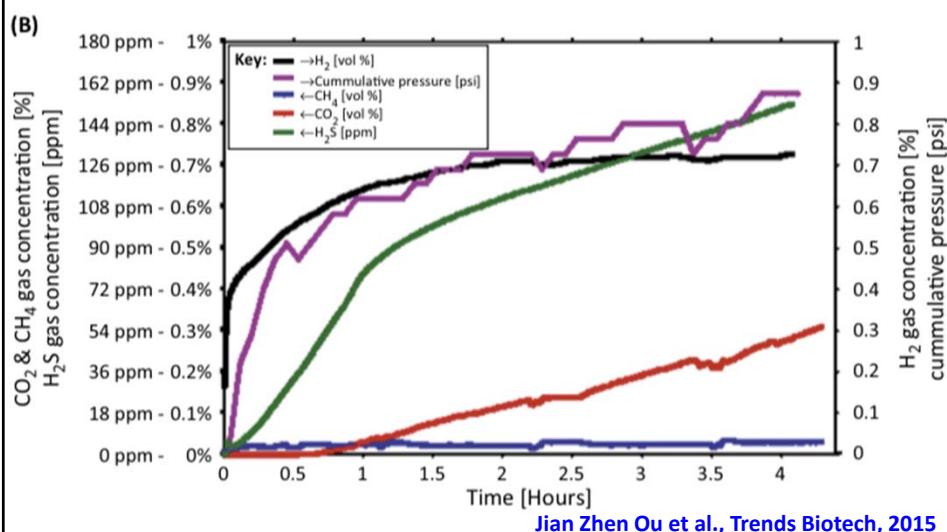

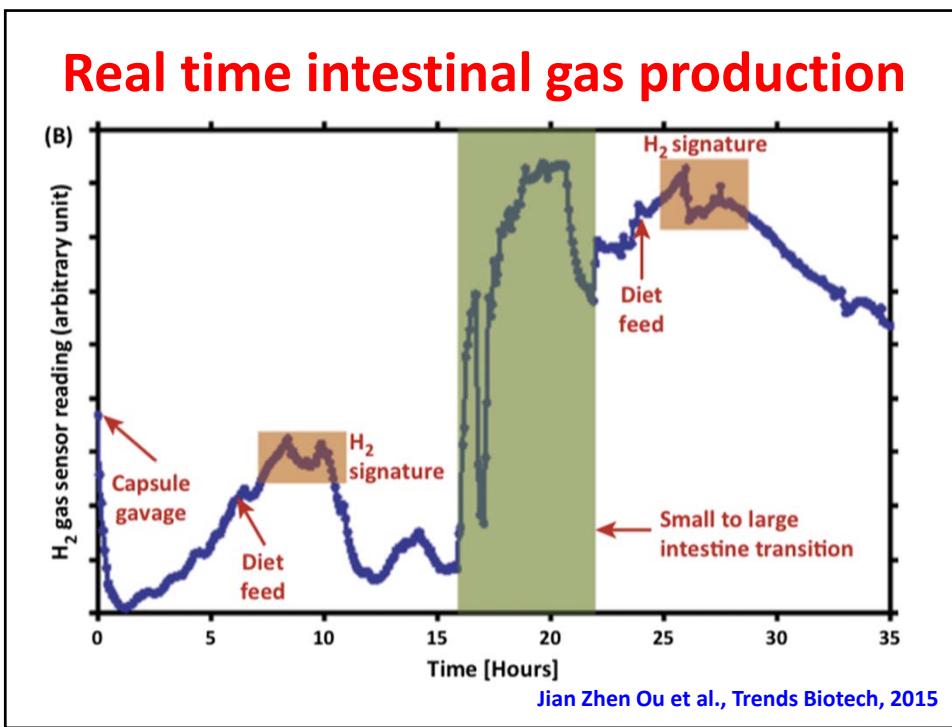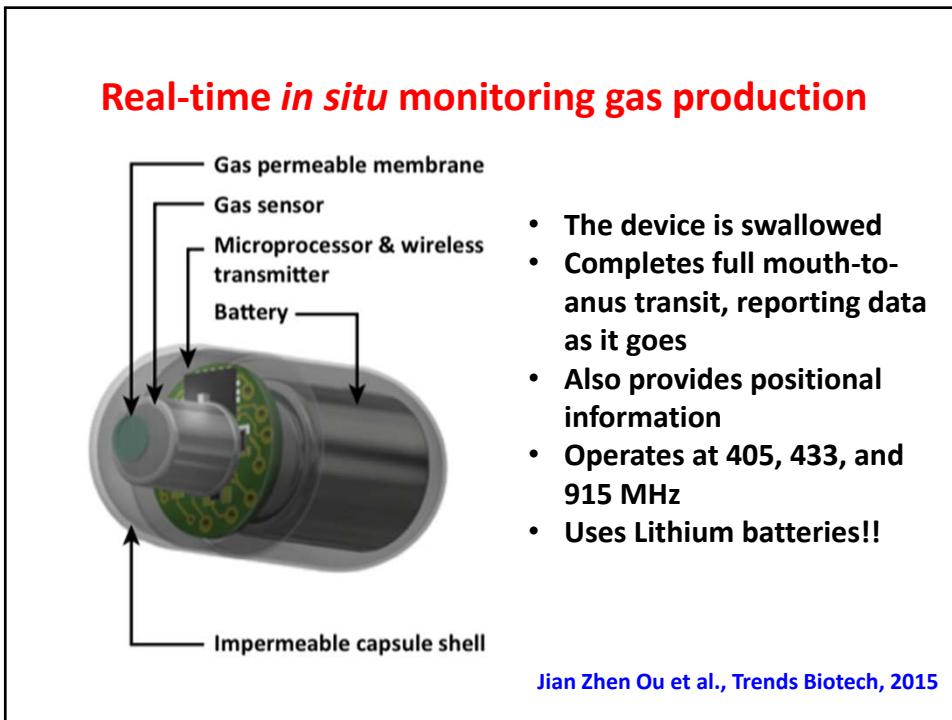


The Challenge for Mass Spec




How to get the mammoth into the gas phase for analysis?


Droplet principle of electrospray

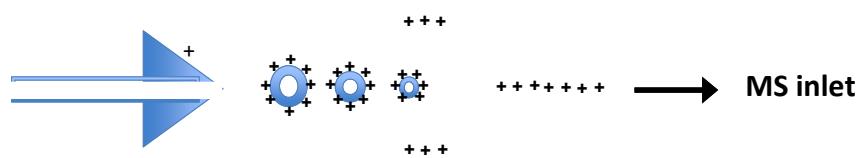

Droplet spray

- Sneeze
- Lung motion
- Surgical knife
- Other vapors



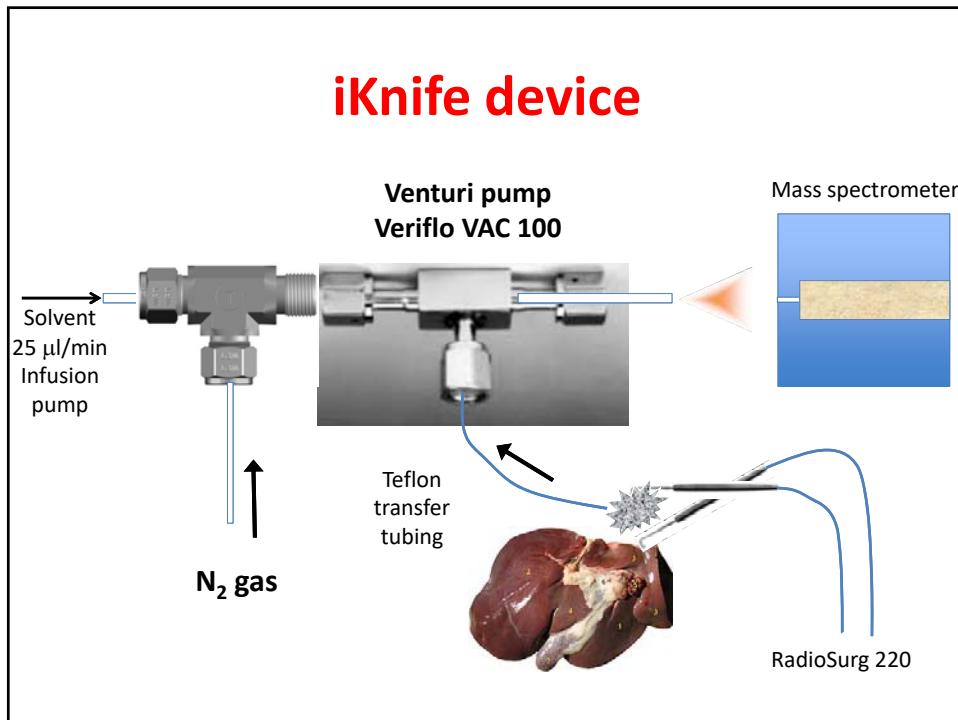

Link to videos by James Kinross


Colorectal surgeon from Imperial College, London
Plenary Speaker at the UAB 2016 Metabolomics Workshop

http://www.uab.edu/proteomics/metabolomics/workshop/2016/videos/kinross_day2.html

http://www.uab.edu/proteomics/metabolomics/workshop/2016/videos/kinross2_day2.html

Mass spectrum of canine stomach


Predominantly phospholipids

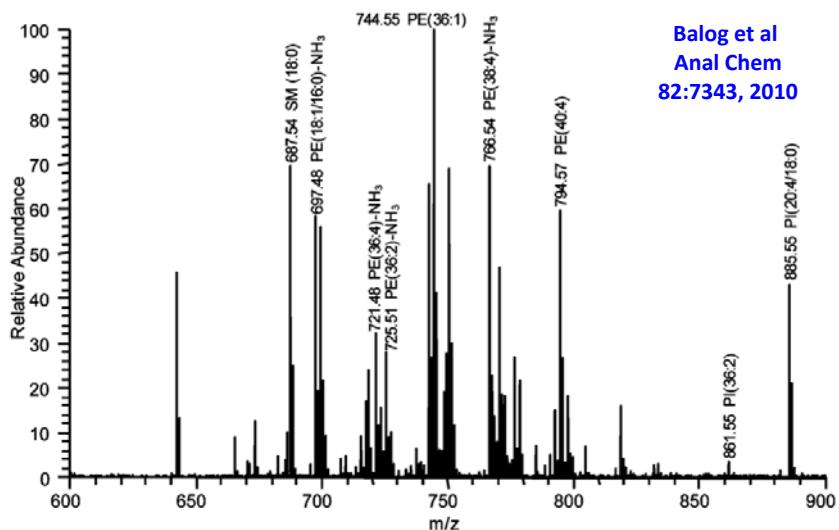


Phospholipid patterns are characteristic of cells and tissues

- Single items are not sufficient as biomarkers
- The classes of phospholipids and their fatty acid composition contain pattern discriminators
- In the absence of known classifiers, principal components analysis looks for groups of components that have the larger sources of variation
 - An individual sample's contributions to these groups are plotted in a 2D or 3D manner


Principal components analysis of ions from surgical “smoke”

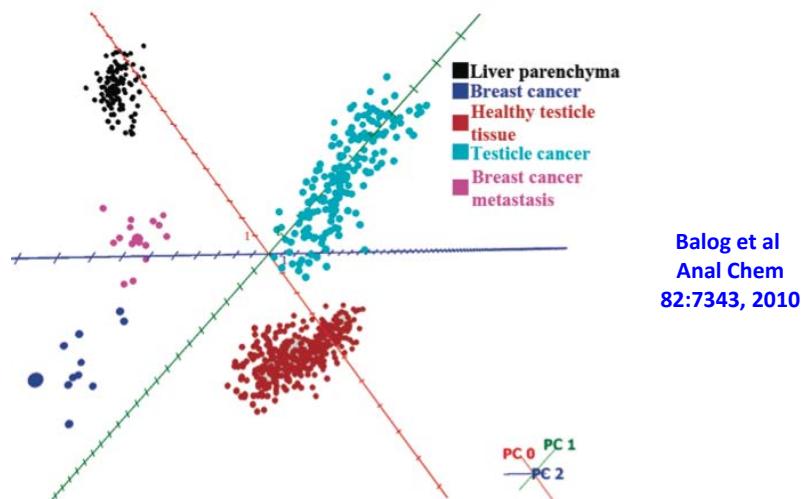

Differentiation of brain tumors

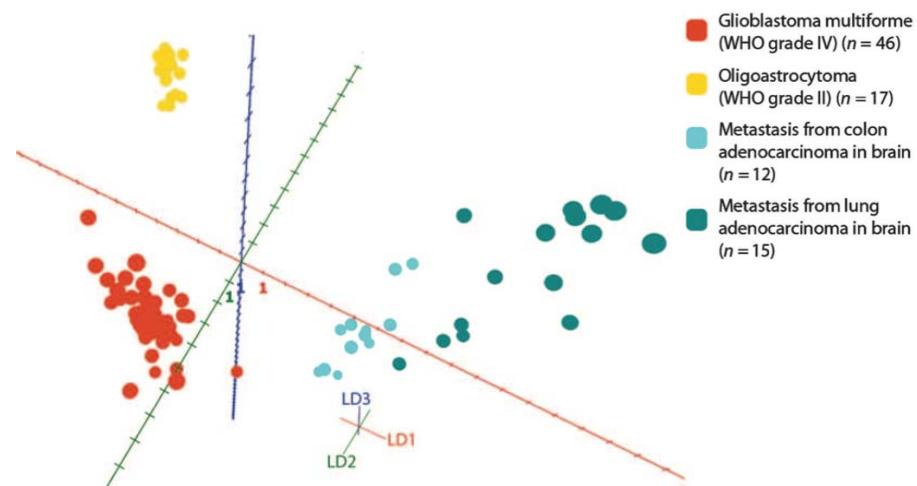


Changing lipids across cancer margin

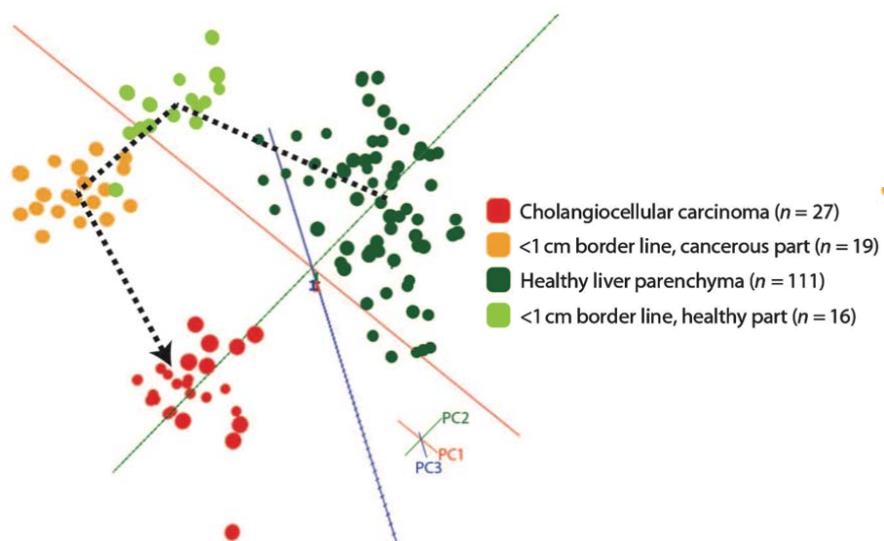

Computer-driven, Rapid Evaporative Imaging MS (REIMS) for tissue sections

Examining tissue (slices) by REIMS

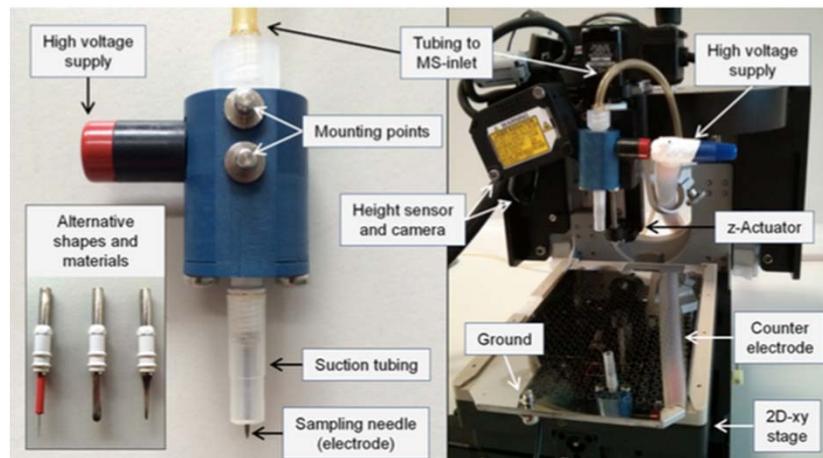


Golf et al., Anal Chem 2015

Modes of data acquisition for REIMS



Line Scans:
Cutting Mode



Individual Pixels:
Pointing Mode

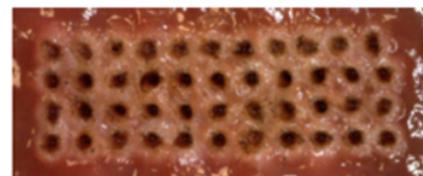


Golf et al., Anal Chem 2015

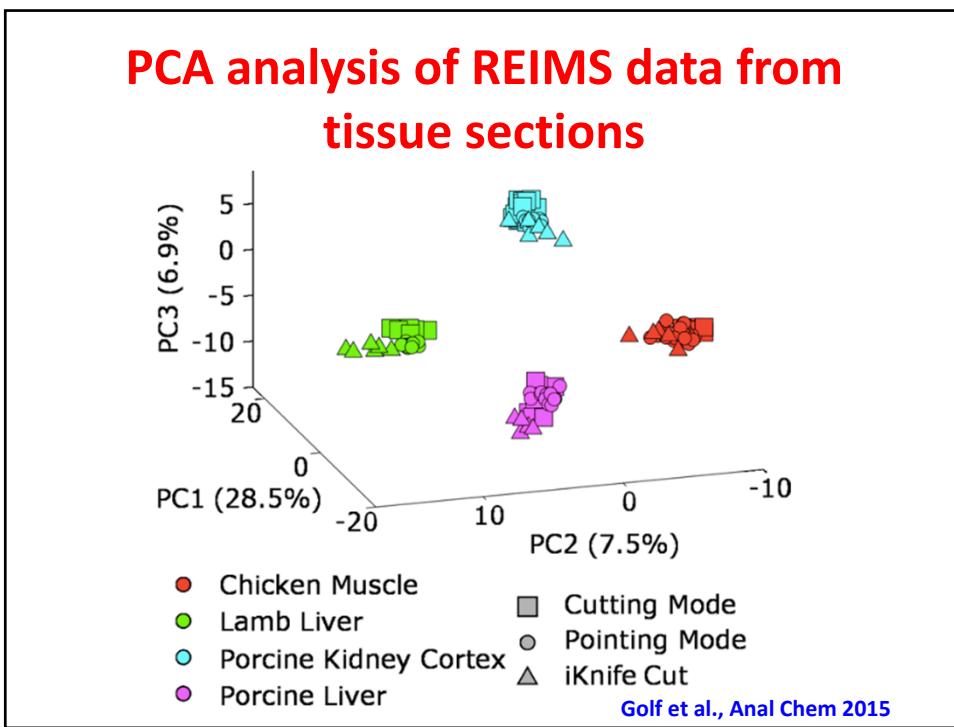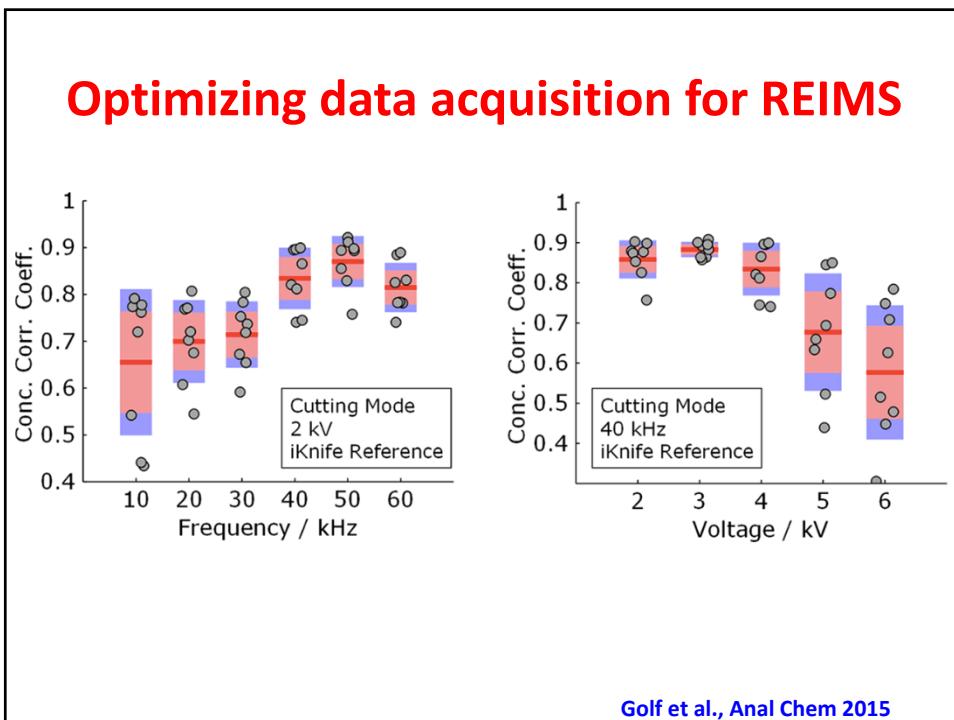



Desorption electrospray ionization (DESI)



- Works by directing an electrical fine spray at a tissue target – does not require deposition of a matrix


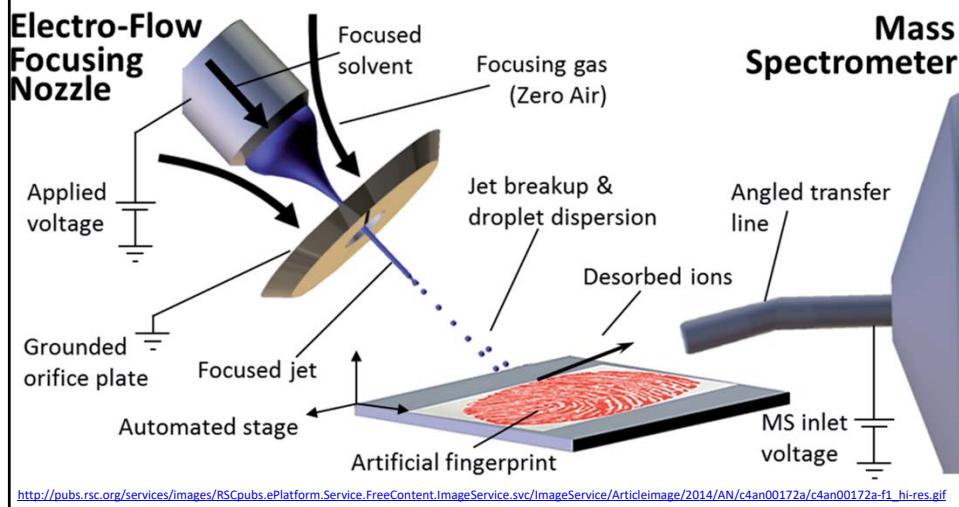




The IDH story of brain and other tumors



- IDH1 (isocitrate dehydrogenase) is mutated in position 132 in a GWAS study of patients with glioblastomas
- IDH1 catalyzes the conversion of isocitrate to alpha-ketoglutarate (α KG) which is a two-step reaction
- Mutant IDH1 catalyzes the first step – to 2-hydroxyglutarate (2HG), but not the second one to α KG
- 2HG is considered to be an onco-metabolite
- What follows is a study from a group at Harvard – performed in the Advanced Multimodality Image Guided Operating Suite at Brigham and Women's Hospital

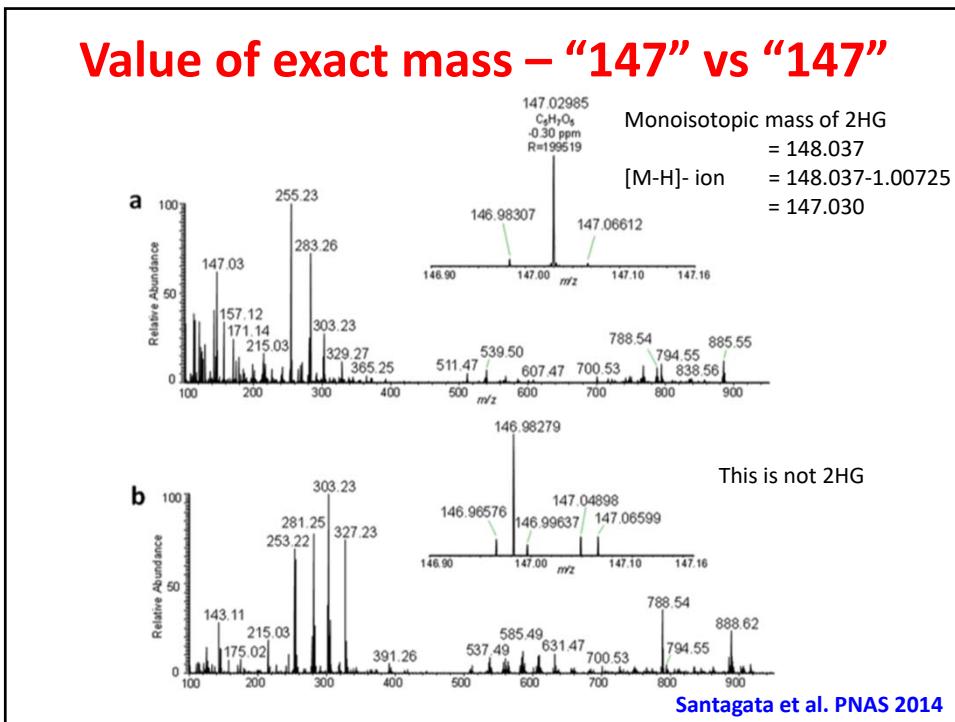
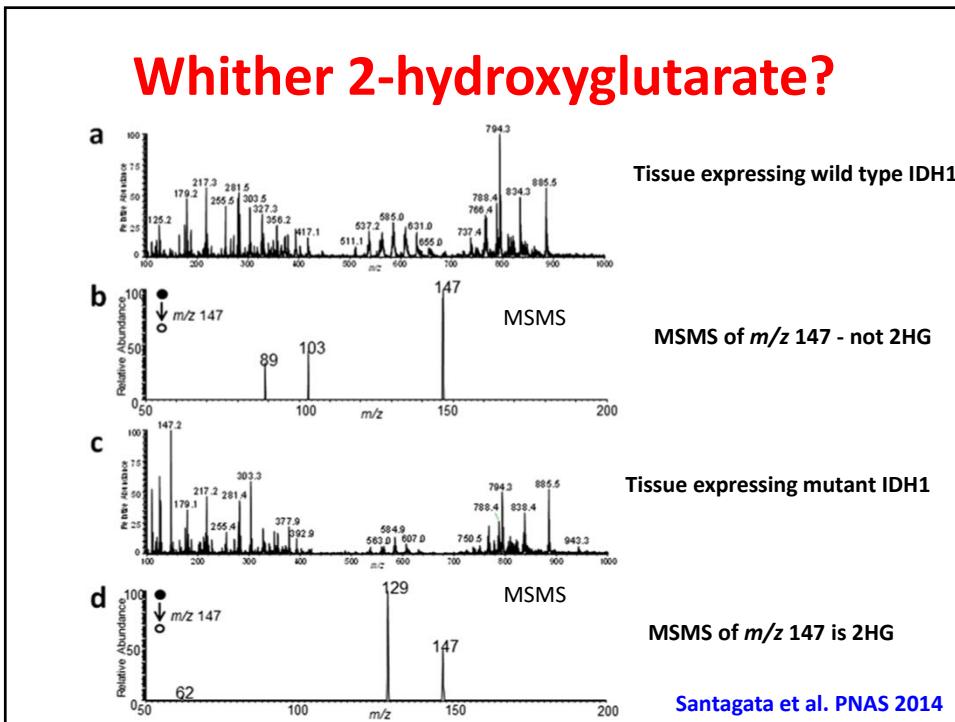


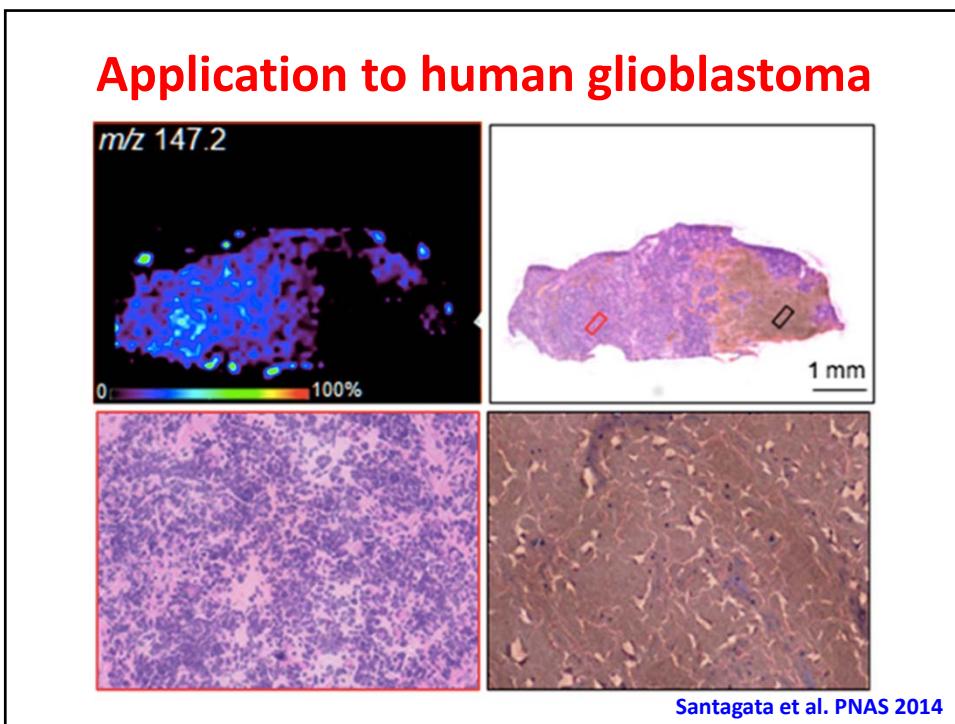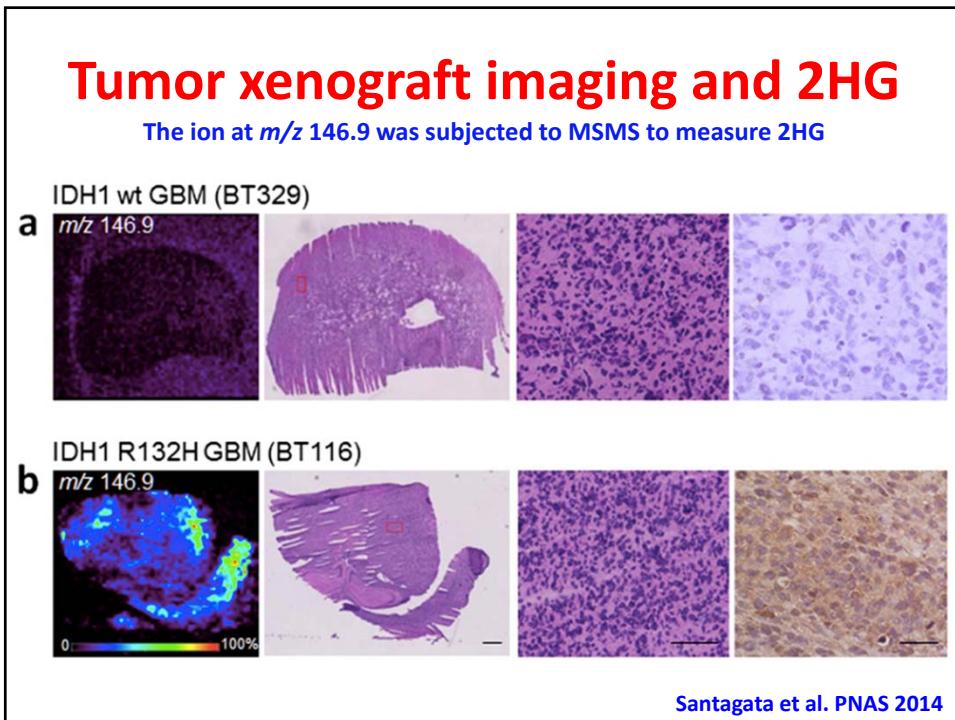

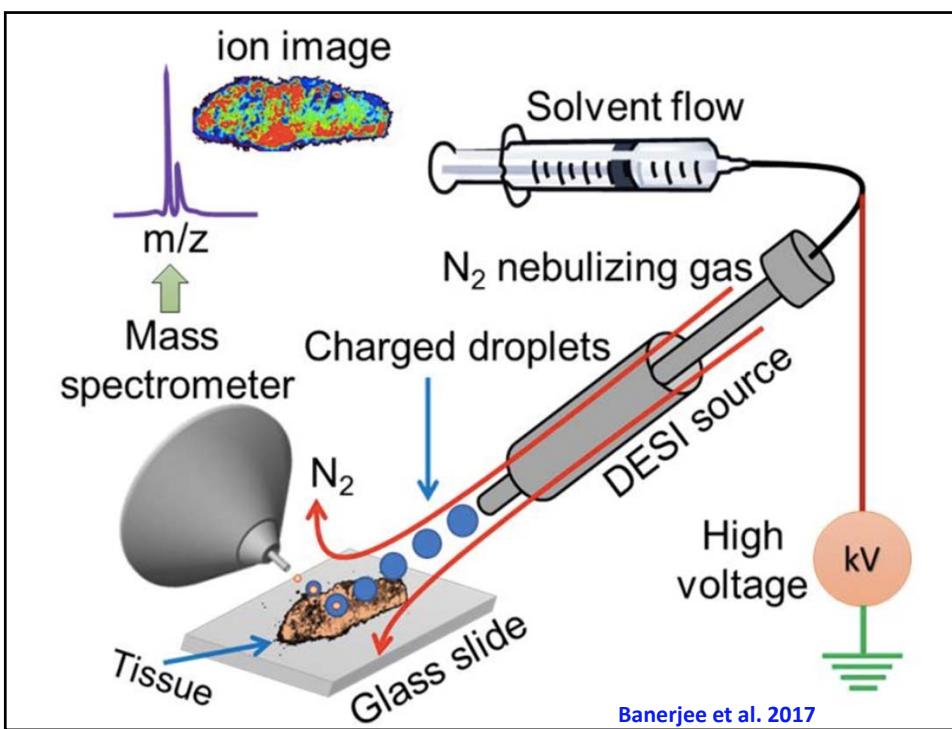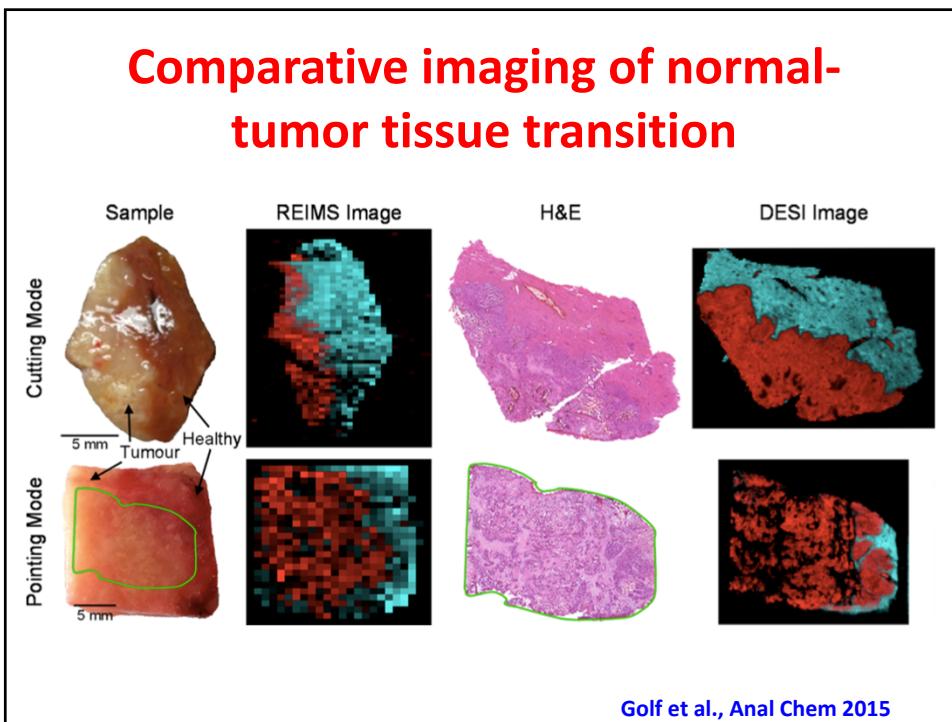

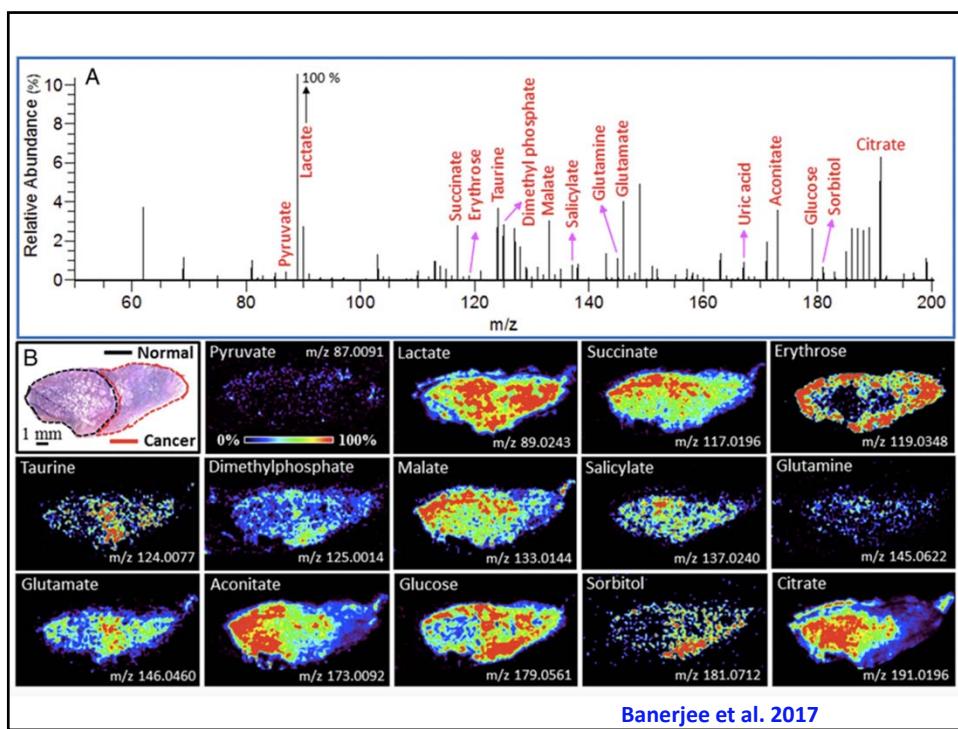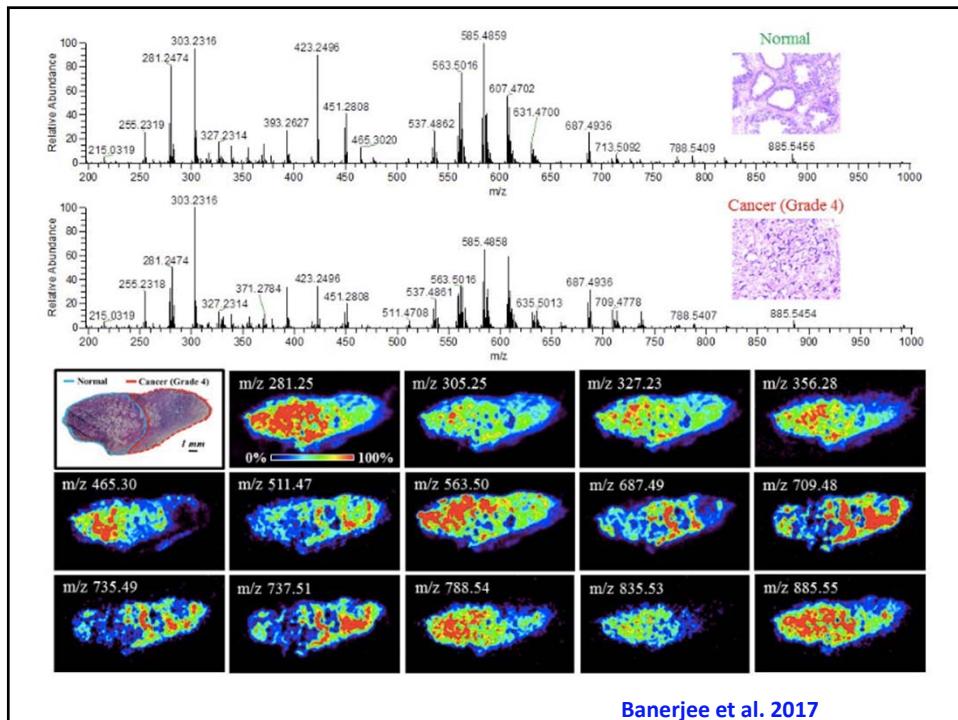

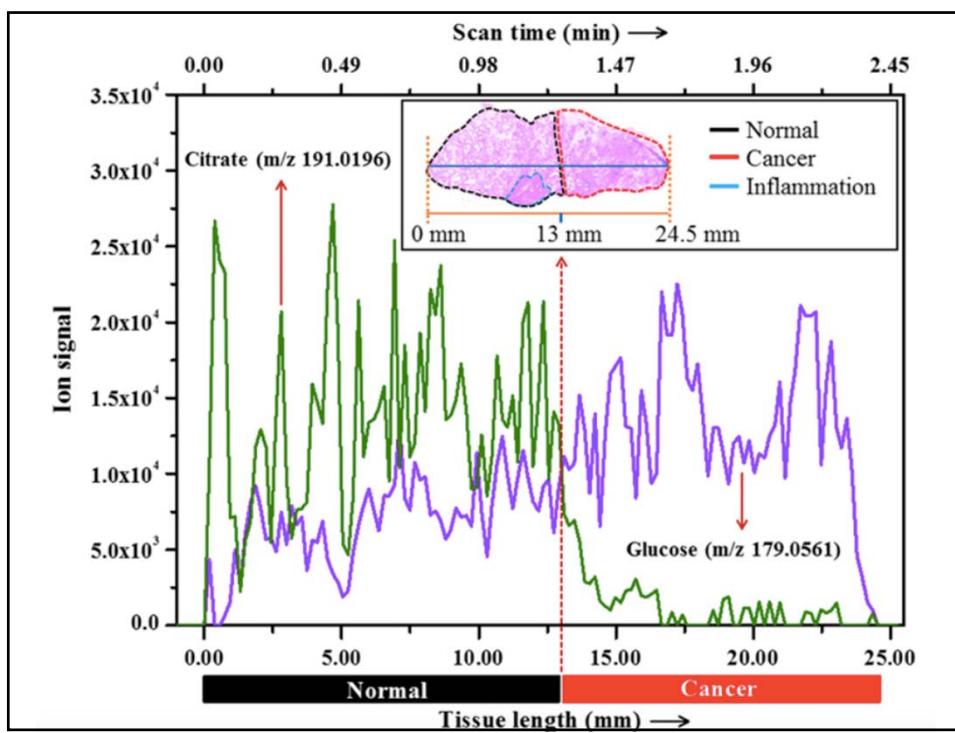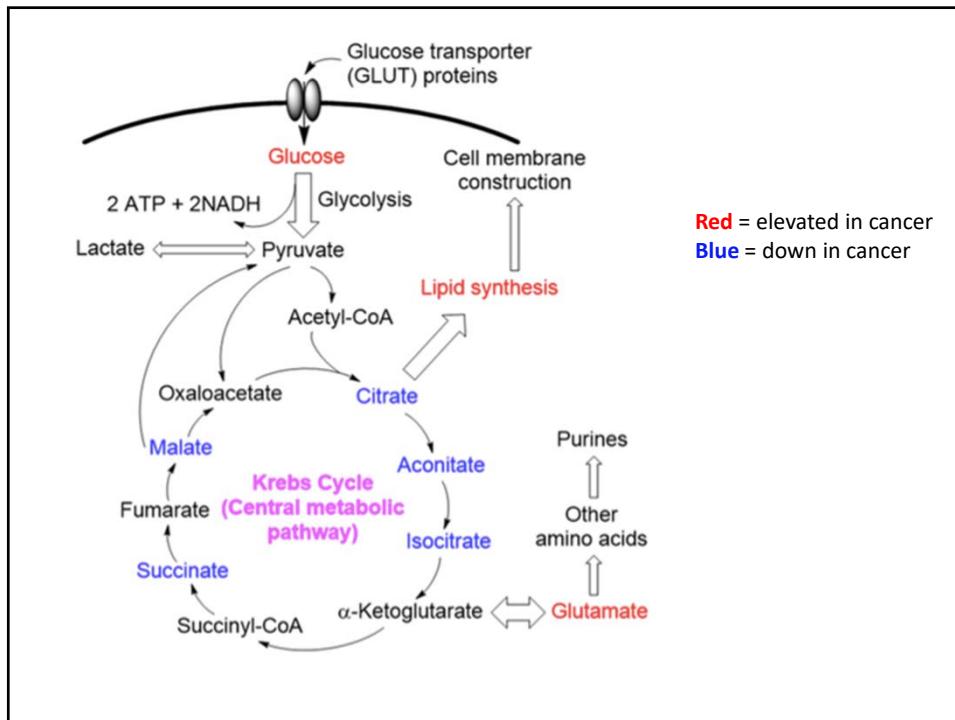

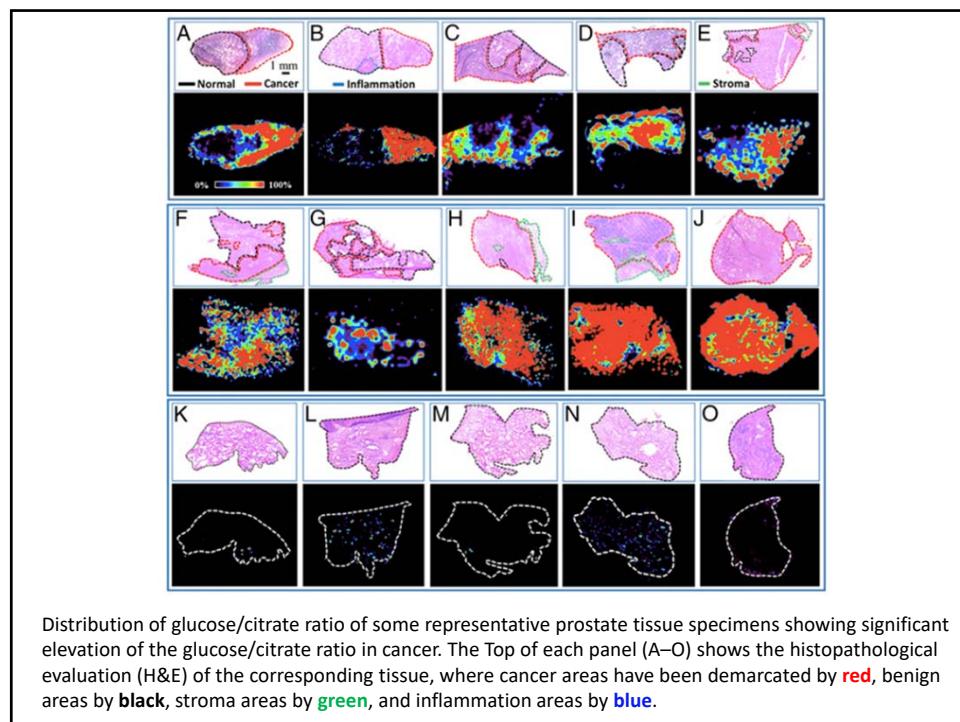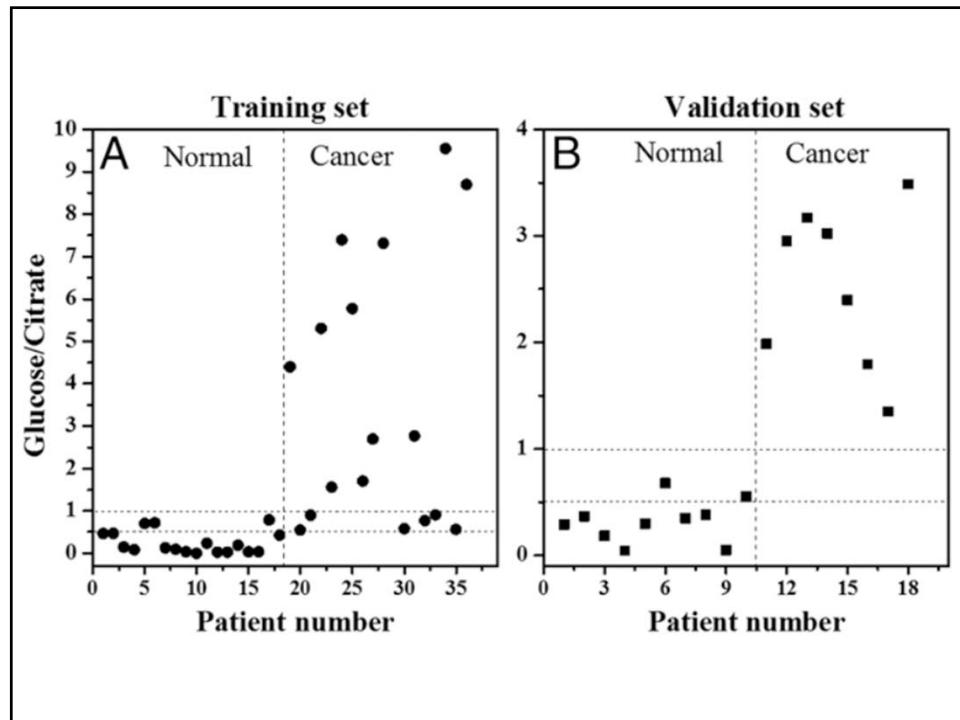

Use of Raman spectroscopy Real-time imaging of metabolites in skin

- <http://bernstein.harvard.edu/research/cars-why.htm>



Sunny Xie, PhD - Harvard

The future of medicine and surgery

<http://www1.imperial.ac.uk/phenomecentre/>

Publications

- Santagata S, Eberlin LS, Norton I, Calligaris D, Feldman DR, Ide JL, Liu X, Wiley JS, Vestal ML, Ramkissoon SH, Orringer DA, Gill KK, Dunn IF, Dias-Santagata D, Ligon KL, Jolesz FA, Golby AJ, Cooks RG, Agar NY. [Intraoperative mass spectrometry mapping of an onco-metabolite to guide brain tumor surgery.](#) PNAS 2014;111(30):11121-6.
- Banerjee S, Zarea RN, Tibshirani RJ, Kunder CA, Nolley R, Fan R, Brooks JD, Sonn GA. Diagnosis of prostate cancer by desorption electrospray ionization mass spectrometric imaging of small metabolites and lipids. [PNAS early edition, March 2017](#)
- Golf O, Strittmatter N, Karancsi T, Pringle SD, Speller AV, Mroz A, Kinross JM, Abbassi-Ghadi N, Jones EA, Takats Z. Rapid evaporative ionization mass spectrometry imaging platform for direct mapping from bulk tissue and bacterial growth media. [Anal Chem. 2015 Mar 3;87\(5\):2527-34.](#)
- In vivo endoscopic tissue identification by rapid evaporative ionization mass spectrometry (REIMS). Balog J, Kumar S, Alexander J, Golf O, Huang J, Wiggins T, Abbassi-Ghadi N, Enyedi A, Kacska S, Kinross J, Hanna GB, Nicholson JK, Takats Z. [Angew Chem Int Ed Engl. 2015 Sep 14;54\(38\):11059-62.](#)